



SEA-BIRD
SCIENTIFIC

SBE Sea-Bird
Electronics

Sea-Bird Electronics
13431 NE 20th Street
Bellevue, Washington
98005 USA

Tel: +1 425-643-9866
seabird@seabird.com
www.seabird.com

SBE41-CP ALACE

Instrument Configuration

Instrument Serial Number: 41-7303
 Instrument Firmware Version: ALACE-CP V 3.0C
 Zero Conductivity Frequency: 2796.69
 Communications Format: RS232
 Communications Settings: 9600 baud, 8 Data Bits, No Parity

Installed Devices/Sensors

<i>Data Format</i>	<i>Measurement</i>	<i>Sensor Type</i>	<i>Serial Number</i>	<i>Rating</i>
Count	Temperature	Internal	N/A	N/A
Frequency	Conductivity	Internal	N/A	N/A
Count	Pressure	Kistler	4645056	2000m(2000 dBar)

CAUTION - This instrument is not intended for underwater use

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 7303
CALIBRATION DATE: 09-Jun-15

SBE 41 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

COEFFICIENTS:


a0 = 7.039563e-005
a1 = 2.697455e-004
a2 = -2.133711e-006
a3 = 1.436325e-007

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	660429.8	1.0000	0.0000
4.5000	563398.0	4.5000	-0.0000
15.0000	356738.7	14.9999	-0.0001
18.5000	308255.0	18.5002	0.0002
23.9940	246568.2	23.9940	-0.0000
29.0000	202412.5	28.9999	-0.0001
32.5000	176916.5	32.5001	0.0001

Temperature ITS-90 = $1 / \{ a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)] \} - 273.15$ (°C)

Residual = instrument temperature - bath temperature

n = instrument output

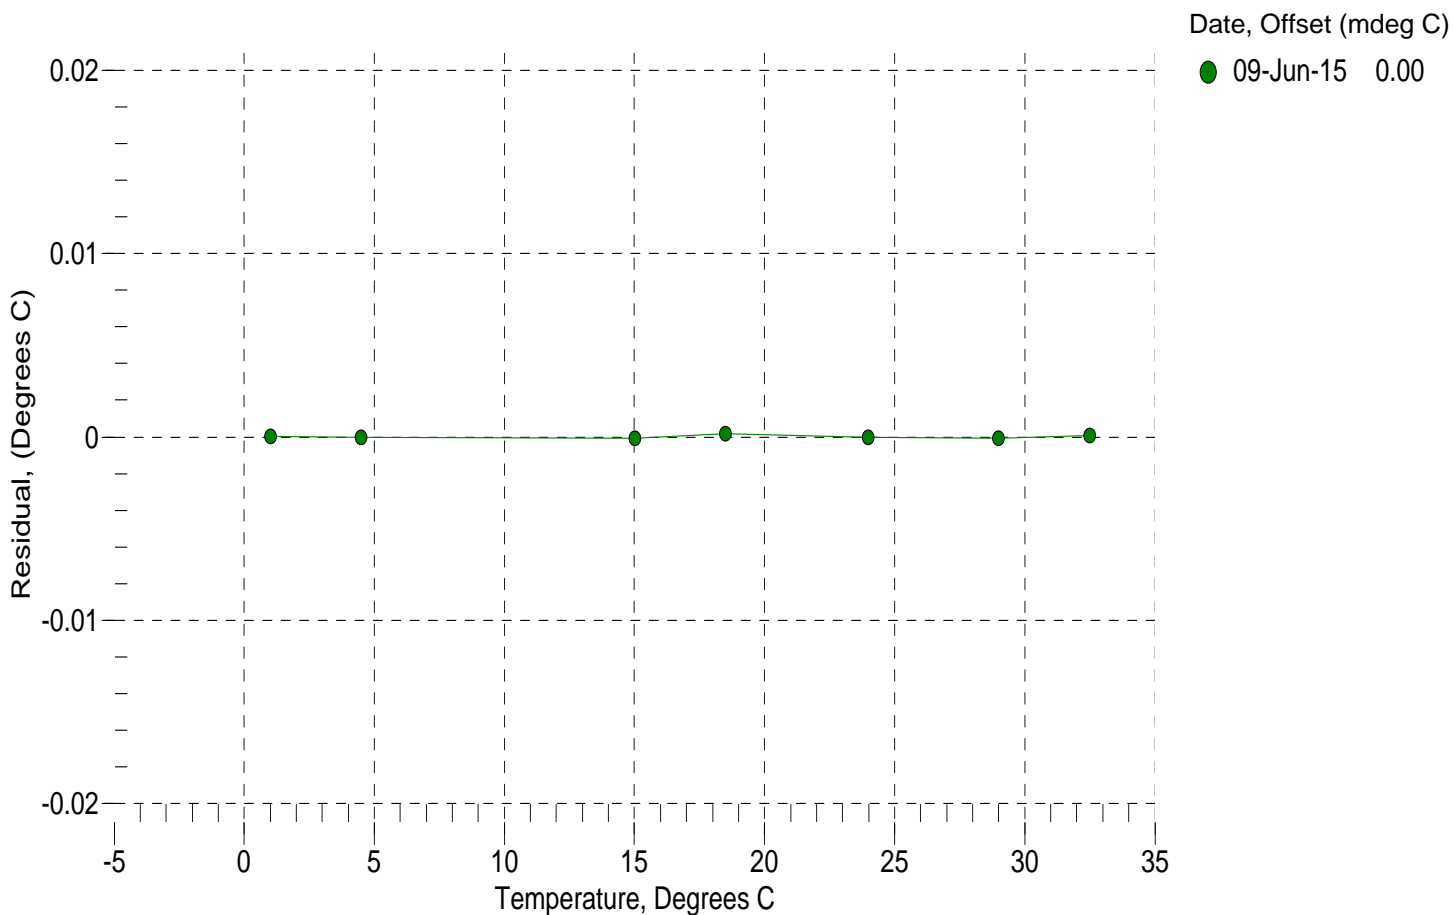

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 7303
CALIBRATION DATE: 09-Jun-15

SBE 41 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -9.954533e-001
h = 1.278111e-001
i = -2.963218e-004
j = 3.685574e-005

CPcor = -9.5700e-008
CTcor = 3.2500e-006
WBOTC = 2.6814e-007


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (Hz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2796.69	0.00000	0.00000
1.0000	34.8842	2.98121	5589.02	2.98122	0.00001
4.5000	34.8647	3.28884	5800.59	3.28884	-0.00000
15.0000	34.8228	4.27233	6429.63	4.27232	-0.00001
18.5000	34.8139	4.61808	6636.33	4.61808	-0.00000
23.9940	34.8043	5.17642	6956.80	5.17643	0.00001
29.0000	34.7992	5.69983	7243.98	5.69983	0.00000
32.5000	34.7966	6.07294	7441.71	6.07294	-0.00001

$$f = \text{INST FREQ} * \text{sqrt}(1.0 + \text{WBOTC} * t) / 1000.0$$

$$\text{Conductivity} = (g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \epsilon * p) \text{ Siemens / meter}$$

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = instrument conductivity - bath conductivity

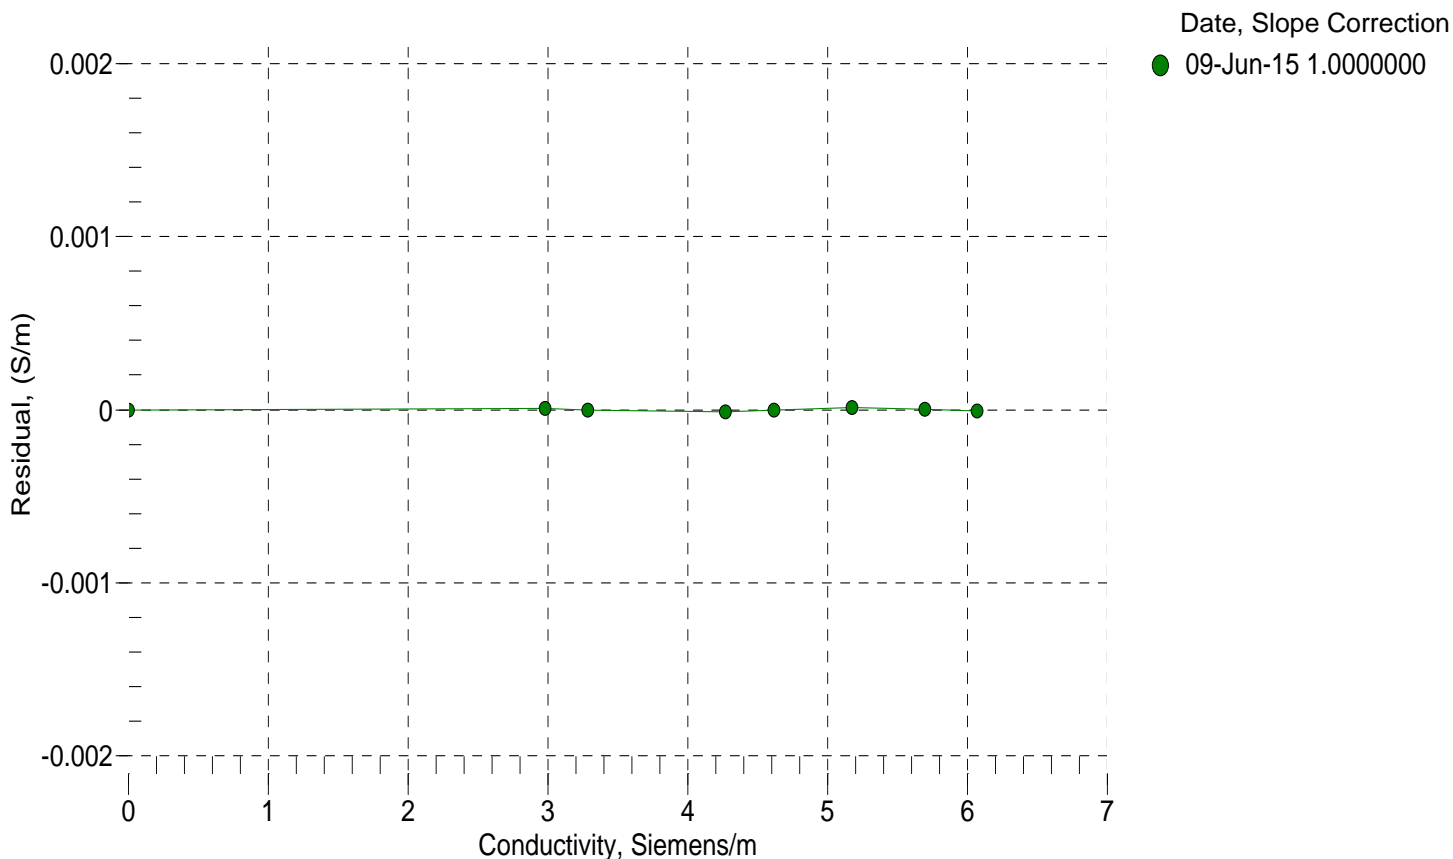

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 7303
CALIBRATION DATE: 02-Jun-15

SBE 41 PRESSURE CALIBRATION DATA
2900 psia S/N 4645056

COEFFICIENTS:

PA0 = -5.385479e-001	PTCA0 = 3.986561e+001
PA1 = 1.404108e-001	PTCA1 = -6.549885e-001
PA2 = 1.137664e-008	PTCA2 = 2.107586e-002
PTHA0 = -9.693469e+001	PTCB0 = 1.035076e+002
PTHA1 = 4.009358e-002	PTCB1 = -5.060453e-003
PTHA2 = 1.192714e-006	PTCB2 = 0.000000e+000

PRESSURE SPAN CALIBRATION

PRESSURE PSIA	INST OUTPUT	THERMISTOR OUTPUT	COMPUTED PRESSURE	ERROR %FS
14.61	144.3	2769.7	14.68	0.00
592.34	4252.1	2776.6	592.31	-0.00
1169.84	8356.8	2778.0	1169.91	0.00
1747.18	12457.4	2778.7	1747.32	0.00
2324.55	16554.9	2779.7	2324.67	0.00
2901.95	20648.4	2780.8	2901.85	-0.00
2324.51	16553.8	2780.3	2324.52	0.00
1747.03	12455.1	2780.3	1747.00	-0.00
1169.82	8355.3	2780.7	1169.70	-0.00
592.26	4250.5	2780.6	592.08	-0.01
14.61	144.4	2781.6	14.67	0.00

THERMAL CORRECTION

TEMP ITS90	PRESS TEMP	INST OUTPUT
32.50	2966.50	154.91
29.00	2892.20	152.80
23.99	2785.40	150.45
18.50	2667.60	149.09
15.00	2591.70	148.91
4.50	2364.00	151.39
1.00	2286.90	153.44

TEMP(ITS90)	SPAN(mV)
-3.92	103.53
35.78	103.33

$y = \text{thermistor output}; t = \text{PTHA0} + \text{PTHA1} * y + \text{PTHA2} * y^2$
 $x = \text{pressure output} - \text{PTCA0} - \text{PTCA1} * t - \text{PTCA2} * t^2$
 $n = x * \text{PTCB0} / (\text{PTCB0} + \text{PTCB1} * t + \text{PTCB2} * t^2)$
 $\text{pressure (psia)} = \text{PA0} + \text{PA1} * n + \text{PA2} * n^2$

