

Certificate no: 4330_1575_00091823
Foil batch no: 1206EMProduct: 4330
Calibration date: 07.01.2014Serial no: 1575
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.142	1.05	-121.445	60.23
1	19.963	0.46	208.840	61.17
2	10.103	0.34	531.000	61.91
3	0.909	0.66	810.260	62.52
4	0.911	17.13	810.185	60.19
5	0.913	39.72	810.105	57.36
6	0.905	59.70	810.355	55.12
7	0.892	99.00	810.740	51.30
8	0.883	139.64	810.975	48.00
9	0.876	210.44	811.195	43.41
10	0.866	310.29	811.465	38.62
11	0.855	411.73	811.760	35.06
12	0.850	508.67	811.940	32.44
13	10.287	13.87	525.095	59.02
14	10.205	30.76	527.730	56.11
15	10.134	47.16	530.000	53.59
16	10.084	78.27	531.590	49.51
17	10.044	112.23	532.885	45.86
18	10.026	166.73	533.450	41.30
19	10.018	245.44	533.690	36.53
20	10.016	323.31	533.755	33.12
21	10.019	408.27	533.665	30.35
22	20.129	11.13	203.340	58.02
23	20.046	25.16	206.100	54.67
24	19.969	37.35	208.655	52.12
25	19.913	62.93	210.480	47.63
26	19.871	89.74	211.860	43.88
27	19.849	131.99	212.585	39.35
28	19.821	196.32	213.495	34.46
29	19.818	260.31	213.610	31.10
30	19.814	326.05	213.730	28.56
31	30.146	9.37	-121.555	56.92
32	30.143	20.75	-121.445	53.27
33	30.146	31.19	-121.520	50.39
34	30.149	51.96	-121.645	45.67
35	30.154	73.16	-121.800	41.93
36	30.159	107.91	-121.970	37.32
37	30.168	159.83	-122.230	32.59
38	30.177	212.89	-122.505	29.29
39	30.178	268.21	-122.560	26.84

Certificate no: 4330_1575_00091823
Foil batch no: 1206EM

Product: 4330
Calibration date: 07.01.2014

Serial no: 1575
Page 2 of 2

Index	0	1	2	3	4	5	6
SUVFoilCoef	2.80618E-03	1.19650E-04	2.28948E-06	2.31166E02	-3.28933E-01	-5.50513E01	4.56659E00
TempCoef	2.63306E01	-3.09453E-02	3.10677E-06	-4.48984E-09	0.00000E00	0.00000E00	

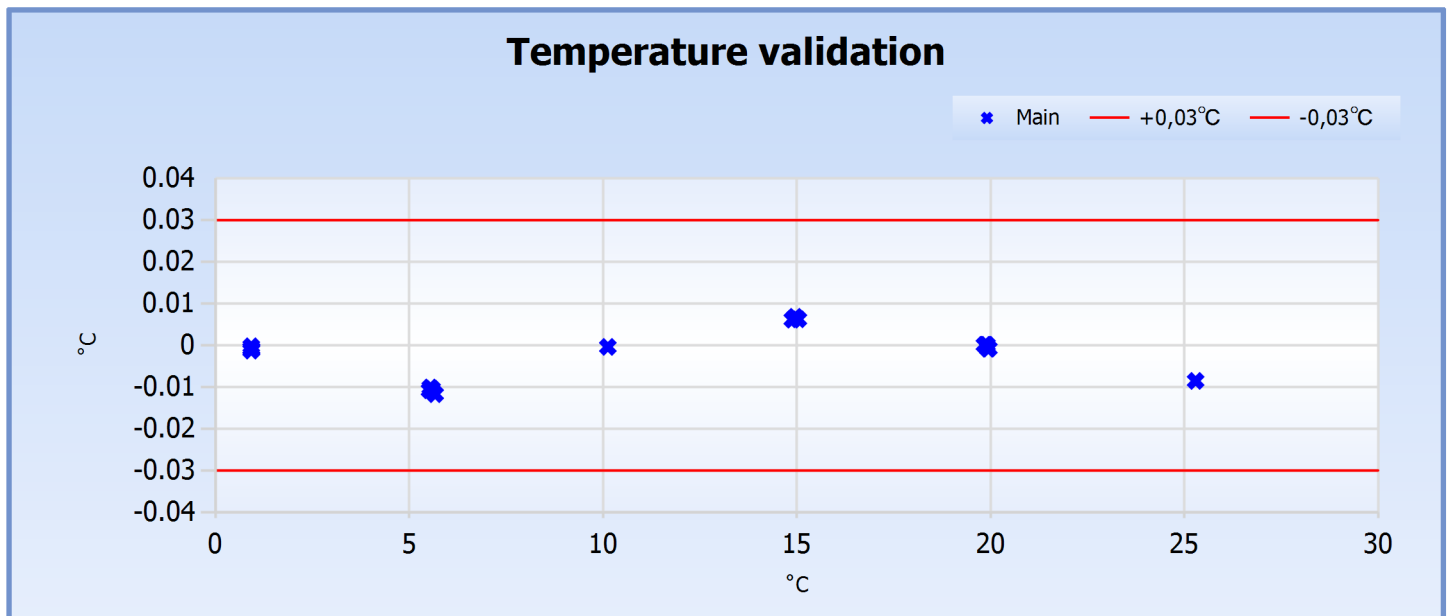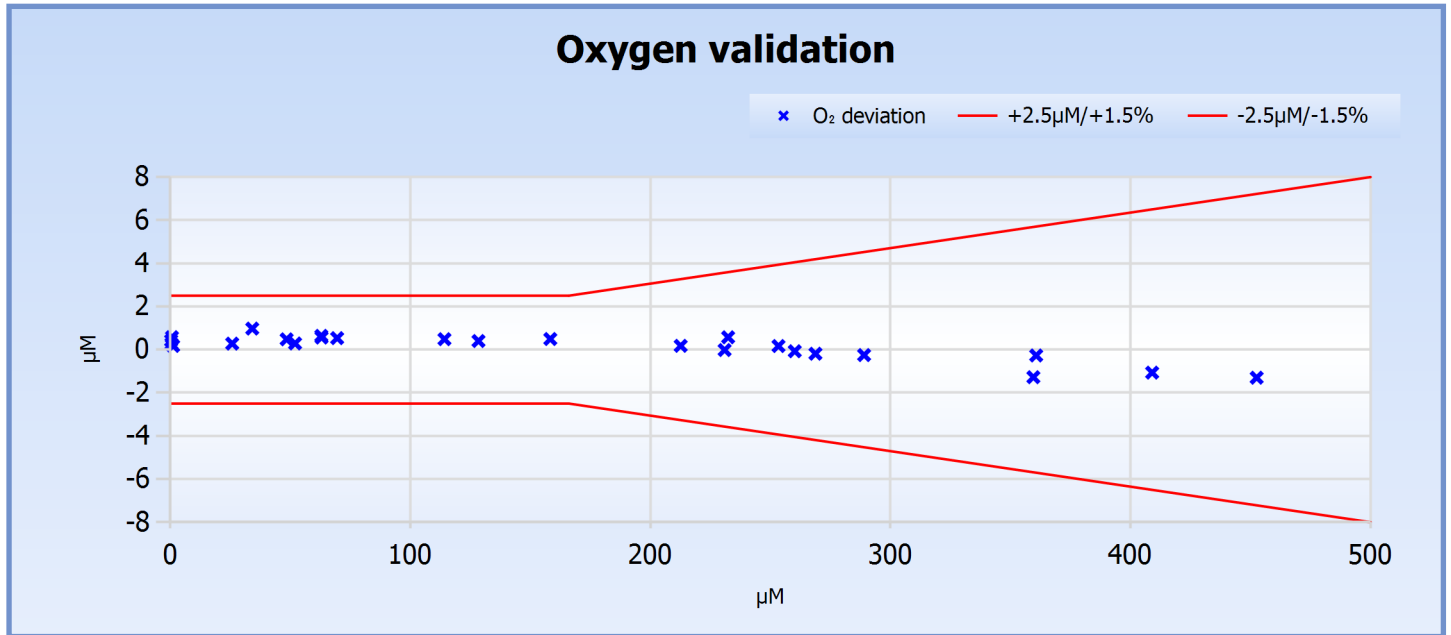

Date:07.01.2014

Tor-Ove Kvalvaag
Tor-Ove Kvalvaag, Calibration Engineer