

Certificate no: 4330_2513_00115020
Foil batch no: 1517MProduct: 4330
Calibration date: 22.01.2016Serial no: 2513
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.148	1.13	-165.150	61.29
1	19.669	0.22	172.275	62.66
2	9.759	0.19	496.390	63.51
3	0.653	0.68	775.860	64.22
4	0.608	20.67	777.150	61.60
5	0.576	40.87	778.065	59.22
6	0.547	60.90	778.905	57.08
7	0.515	101.42	779.820	53.30
8	0.488	143.52	780.600	50.03
9	0.472	214.08	781.075	45.62
10	0.464	317.50	781.295	40.79
11	0.458	421.44	781.495	37.24
12	0.449	525.88	781.710	34.51
13	10.189	13.86	482.605	60.84
14	10.100	31.54	485.480	57.86
15	10.025	47.53	487.855	55.47
16	9.950	79.97	490.300	51.34
17	9.893	112.71	492.105	47.94
18	9.853	168.62	493.400	43.37
19	9.836	250.12	493.920	38.54
20	9.831	331.84	494.100	35.06
21	9.828	415.91	494.200	32.39
22	19.972	10.97	162.245	59.75
23	19.892	24.86	164.895	56.50
24	19.814	37.91	167.455	53.83
25	19.738	64.15	169.970	49.38
26	19.699	90.47	171.245	45.80
27	19.680	134.78	171.895	41.17
28	19.674	199.72	172.100	36.39
29	19.670	266.09	172.200	32.98
30	19.669	335.04	172.205	30.38
31	30.109	8.92	-163.970	58.59
32	30.103	20.33	-163.800	54.98
33	30.105	30.98	-163.820	52.10
34	30.112	52.31	-164.020	47.38
35	30.122	73.66	-164.370	43.69
36	30.133	109.48	-164.700	39.05
37	30.142	162.89	-164.995	34.30
38	30.145	217.28	-165.055	31.02
39	30.145	274.93	-165.085	28.53

Certificate no: 4330_2513_00115020
Foil batch no: 1517M

Product: 4330
Calibration date: 22.01.2016

Serial no: 2513
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.70832E-03	1.15010E-04	2.35887E-06	2.27770E02	-3.74611E-01	-6.30023E01	4.51610E00
TempCoef	2.49364E01	-3.09544E-02	2.91355E-06	-4.33117E-09	0.00000E00	0.00000E00	

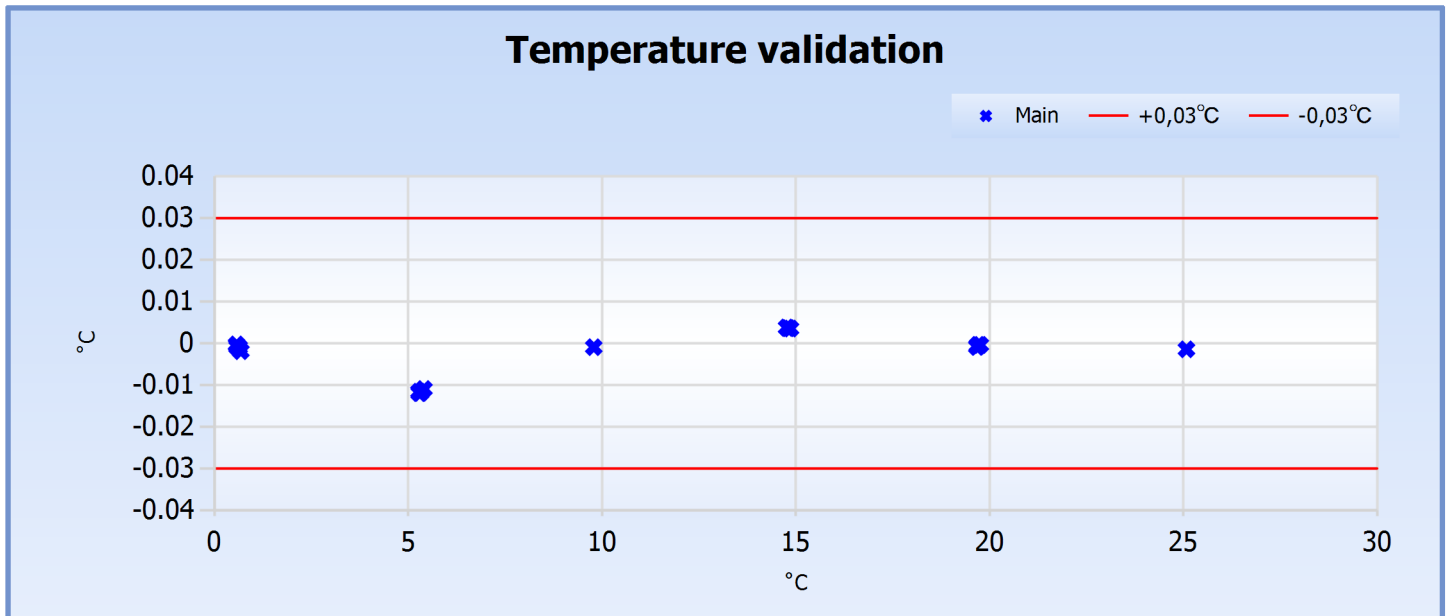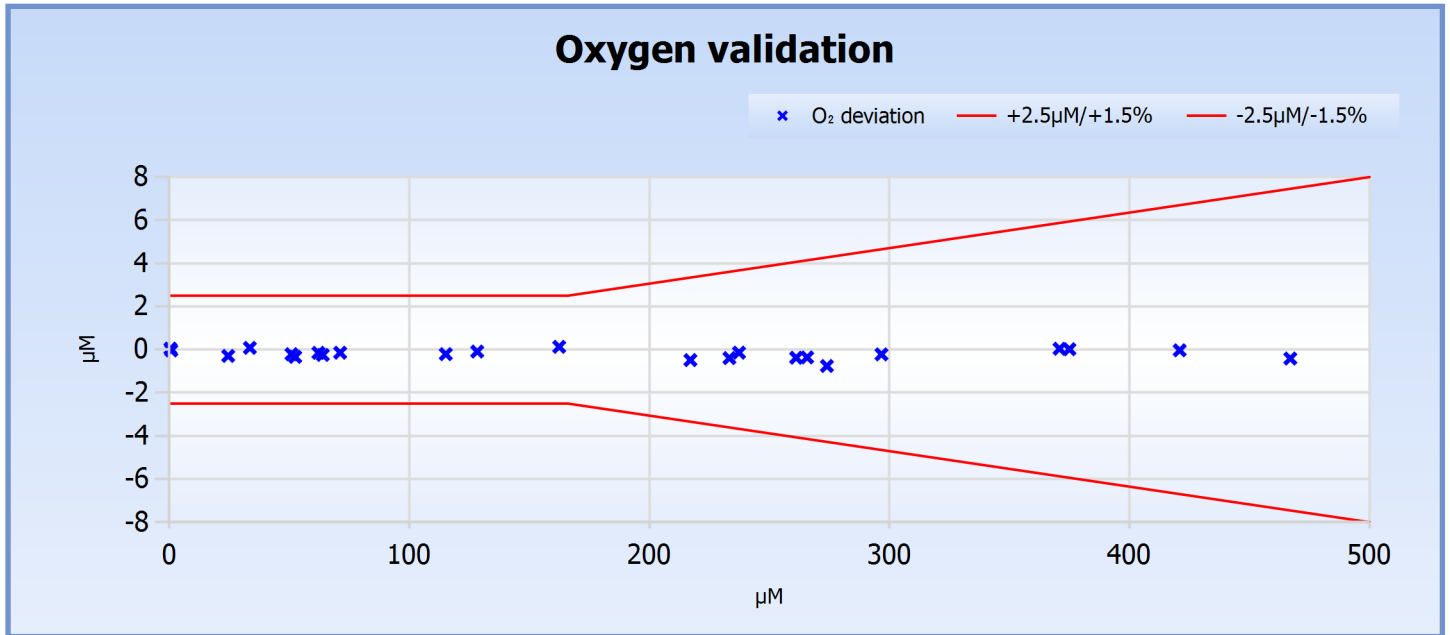

Date:22.01.2016

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer