

Certificate no: 4330_1466_00111916
Foil batch no: 1206EMProduct: 4330
Calibration date: 18.10.2015Serial no: 1466
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.053	1.96	-135.400	61.61
1	19.744	1.19	201.400	62.82
2	9.804	1.40	529.240	63.57
3	0.699	2.23	808.405	64.21
4	0.675	20.28	809.135	61.33
5	0.664	43.94	809.450	58.01
6	0.654	64.77	809.735	55.44
7	0.639	107.87	810.155	50.96
8	0.631	150.41	810.390	47.37
9	0.626	219.82	810.515	42.79
10	0.619	328.49	810.725	37.66
11	0.616	429.61	810.825	34.26
12	0.612	533.80	810.945	31.60
13	10.080	14.38	520.330	60.50
14	10.016	34.20	522.425	56.60
15	9.969	50.41	523.945	53.85
16	9.934	84.66	525.060	49.04
17	9.915	118.16	525.670	45.33
18	9.901	174.09	526.125	40.59
19	9.881	253.39	526.755	35.83
20	9.877	341.93	526.900	32.16
21	9.884	422.13	526.660	29.70
22	19.985	11.69	193.360	59.37
23	19.889	27.23	196.575	55.14
24	19.817	40.11	198.960	52.21
25	19.765	66.94	200.685	47.22
26	19.734	94.06	201.730	43.34
27	19.712	138.30	202.460	38.59
28	19.689	202.04	203.220	33.89
29	19.684	268.49	203.395	30.53
30	19.681	335.46	203.500	28.07
31	30.028	9.66	-134.600	58.26
32	30.043	22.19	-135.065	53.71
33	30.055	32.79	-135.435	50.52
34	30.060	54.17	-135.600	45.42
35	30.066	75.43	-135.775	41.56
36	30.068	111.77	-135.880	36.73
37	30.073	163.27	-136.015	32.15
38	30.079	219.98	-136.190	28.77
39	30.084	275.15	-136.370	26.45

Certificate no: 4330_1466_00111916
 Foil batch no: 1206EM

Product: 4330
 Calibration date: 18.10.2015

Serial no: 1466
 Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	3.23457E-03	1.38191E-04	2.57306E-06	2.33376E02	-3.22120E-01	-5.87930E01	4.52191E00
TempCoef	2.58324E01	-3.06733E-02	3.09582E-06	-4.46639E-09	0.00000E00	0.00000E00	

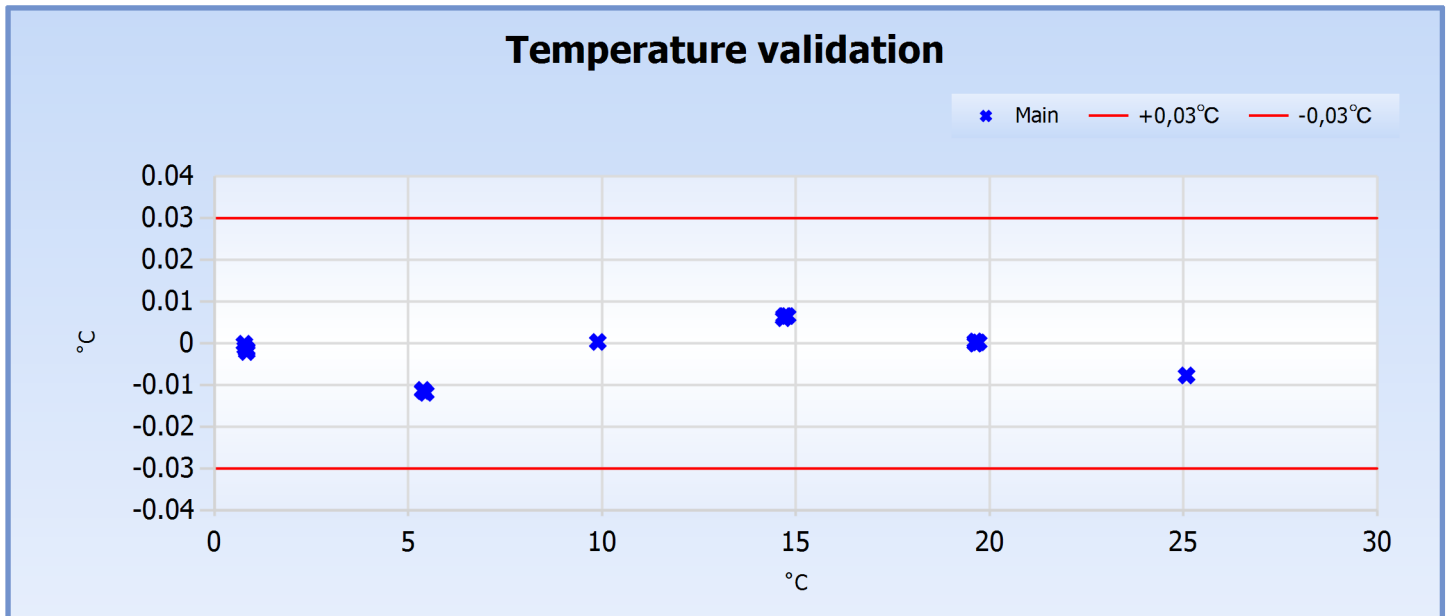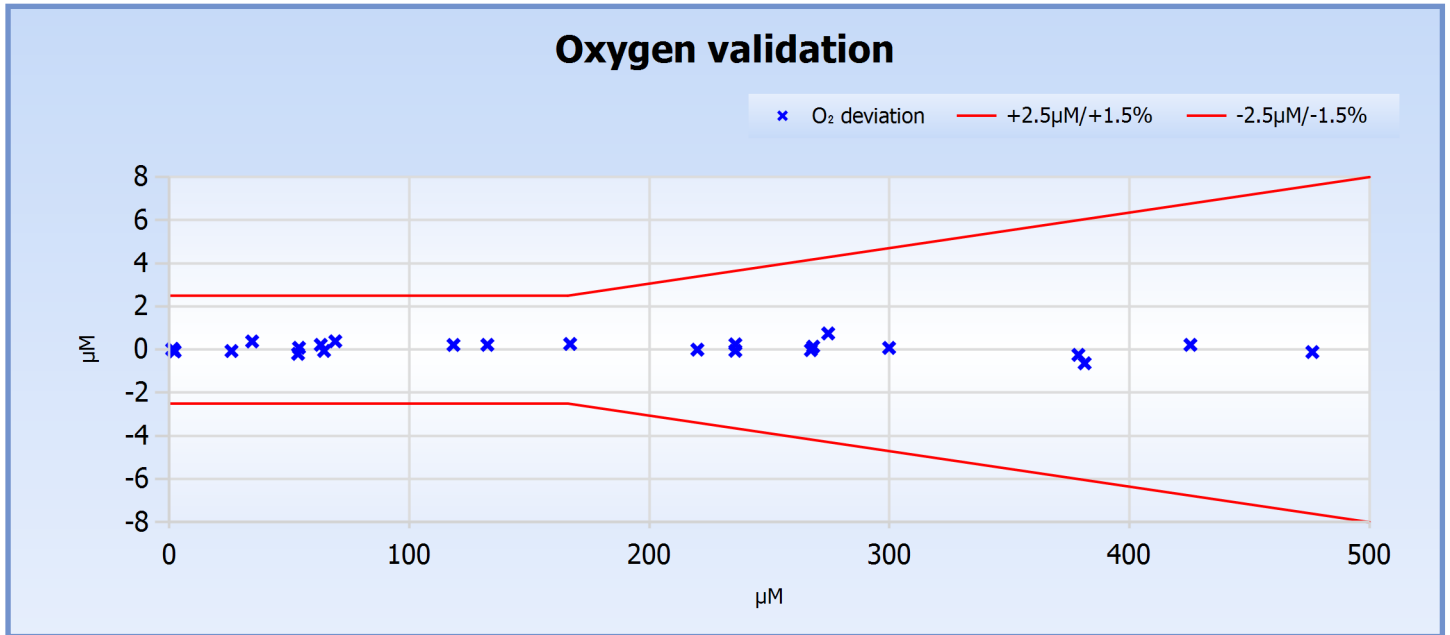

Date: 18.10.2015


 Tor-Ove Kvalvaag, Calibration Engineer