

Certificate no: 4330_2520_00115024
Foil batch no: 1517M

Product: 4330
Calibration date: 22.01.2016

Serial no: 2520
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.148	1.13	-50.235	59.15
1	19.669	0.22	283.155	60.36
2	9.759	0.19	594.885	61.15
3	0.653	0.68	857.415	61.79
4	0.608	20.67	858.630	59.13
5	0.576	40.87	859.490	56.70
6	0.547	60.90	860.270	54.53
7	0.515	101.42	861.120	50.71
8	0.488	143.52	861.830	47.39
9	0.472	214.08	862.300	42.94
10	0.464	317.50	862.500	38.10
11	0.458	421.44	862.675	34.53
12	0.449	525.88	862.900	31.80
13	10.189	13.86	581.800	58.47
14	10.100	31.54	584.515	55.43
15	10.025	47.53	586.800	53.00
16	9.950	79.97	589.115	48.81
17	9.893	112.71	590.840	45.36
18	9.853	168.62	592.060	40.75
19	9.836	250.12	592.595	35.88
20	9.831	331.84	592.700	32.40
21	9.828	415.91	592.800	29.72
22	19.972	10.97	273.450	57.33
23	19.892	24.86	276.045	54.04
24	19.814	37.91	278.515	51.35
25	19.738	64.15	280.965	46.86
26	19.699	90.47	282.205	43.27
27	19.680	134.78	282.800	38.61
28	19.674	199.72	283.000	33.81
29	19.670	266.09	283.110	30.40
30	19.669	335.04	283.200	27.81
31	30.109	8.92	-49.040	56.22
32	30.103	20.33	-48.810	52.58
33	30.105	30.98	-48.900	49.67
34	30.112	52.31	-49.100	44.93
35	30.122	73.66	-49.410	41.21
36	30.133	109.48	-49.800	36.55
37	30.142	162.89	-50.030	31.80
38	30.145	217.28	-50.100	28.52
39	30.145	274.93	-50.105	26.03

Certificate no: 4330_2520_00115024
Foil batch no: 1517M

Product: 4330
Calibration date: 22.01.2016

Serial no: 2520
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.76371E-03	1.17642E-04	2.26806E-06	2.31779E02	-3.66485E-01	-5.24763E01	4.58536E00
TempCoef	2.85356E01	-3.19160E-02	3.53705E-06	-4.94800E-09	0.00000E00	0.00000E00	

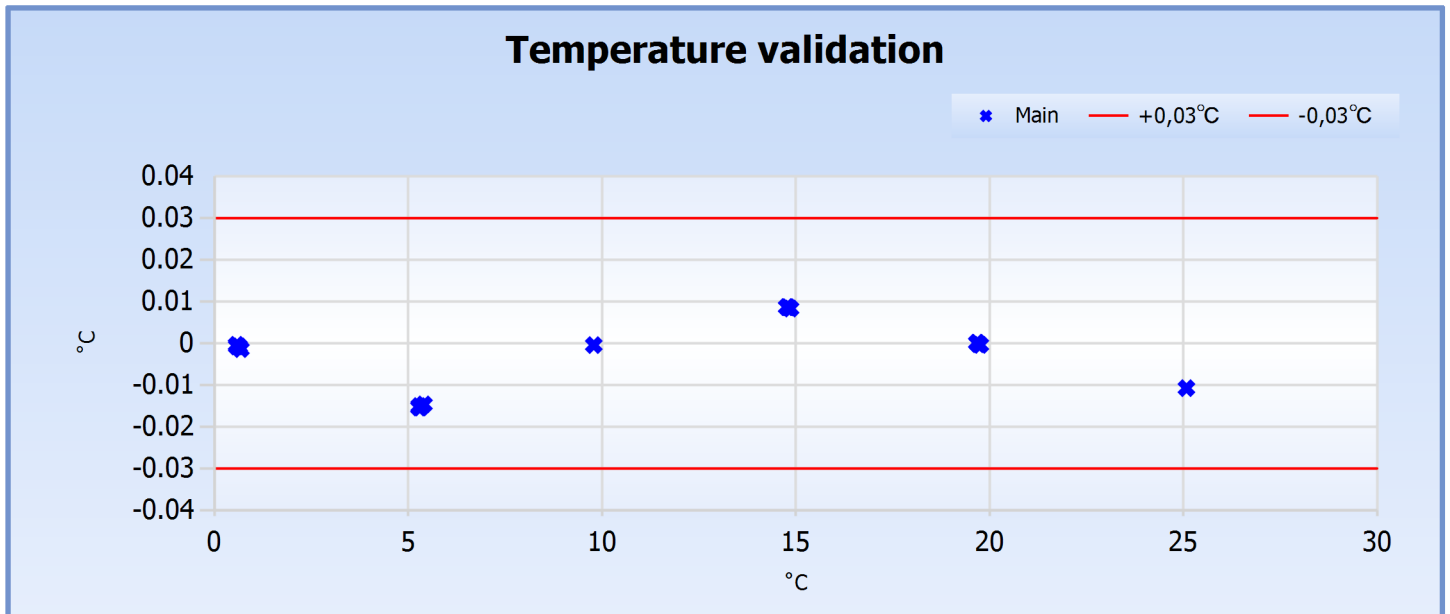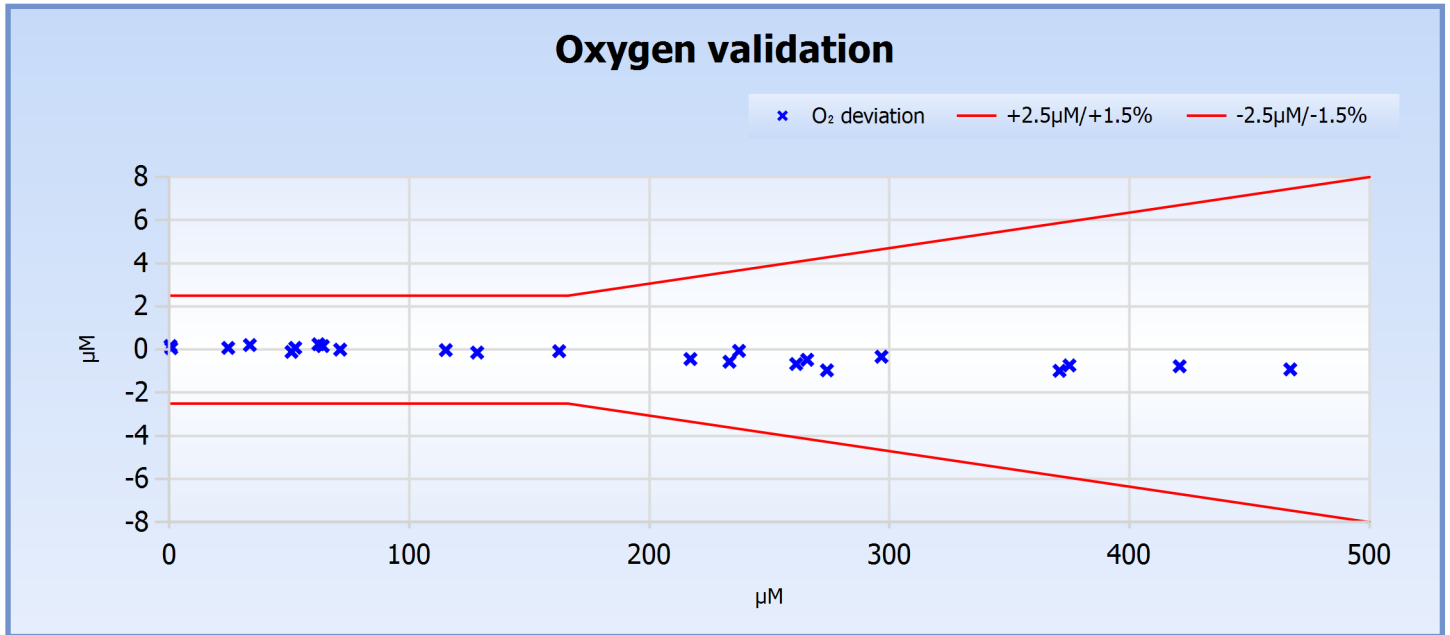

Date:22.01.2016

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer