

Certificate no: 4330\_2935\_00141933  
Foil batch no: 1517M

Product: 4330  
Calibration date: 14.01.2018

Serial no: 2935  
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.285	0.22	-50.100	62.54
1	19.655	0.15	293.893	63.45
2	9.746	0.40	609.907	64.25
3	0.547	1.37	876.800	64.94
4	0.546	21.16	876.853	62.17
5	0.554	44.44	876.607	59.29
6	0.557	66.54	876.513	56.86
7	0.549	107.99	876.773	52.95
8	0.551	151.57	876.693	49.56
9	0.559	225.26	876.493	45.01
10	0.567	324.05	876.247	40.48
11	0.572	434.00	876.127	36.78
12	0.574	549.08	876.067	33.90
13	10.095	12.98	599.207	61.75
14	10.023	32.51	601.400	58.25
15	9.965	49.91	603.160	55.54
16	9.924	83.85	604.440	51.14
17	9.886	116.44	605.593	47.73
18	9.857	172.96	606.527	43.11
19	9.834	252.02	607.233	38.46
20	9.823	335.47	607.553	34.94
21	9.821	420.40	607.627	32.28
22	19.840	9.48	287.887	60.85
23	19.771	24.28	290.120	57.12
24	19.715	37.79	291.987	54.22
25	19.676	64.90	293.227	49.46
26	19.651	93.02	294.020	45.60
27	19.626	136.26	294.840	41.09
28	19.603	201.45	295.607	36.32
29	19.593	267.50	295.913	32.95
30	19.592	336.88	295.940	30.35
31	29.979	7.38	-40.440	59.80
32	29.983	19.64	-40.567	55.62
33	29.987	30.64	-40.680	52.49
34	29.991	51.88	-40.800	47.63
35	29.993	73.64	-40.860	43.81
36	29.990	109.72	-40.787	39.09
37	29.995	163.46	-40.940	34.31
38	30.001	218.96	-41.100	30.98
39	30.002	276.10	-41.167	28.53

Certificate no: 4330\_2935\_00141933  
Foil batch no: 1517M

Product: 4330  
Calibration date: 14.01.2018

Serial no: 2935  
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.85574E-03	1.19974E-04	2.63848E-06	9.24285E08	-1.39110E06	-2.30351E08	1.82334E07
TempCoef	2.87027E01	-3.14078E-02	3.59335E-06	-5.01386E-09	0.00000E00	0.00000E00	

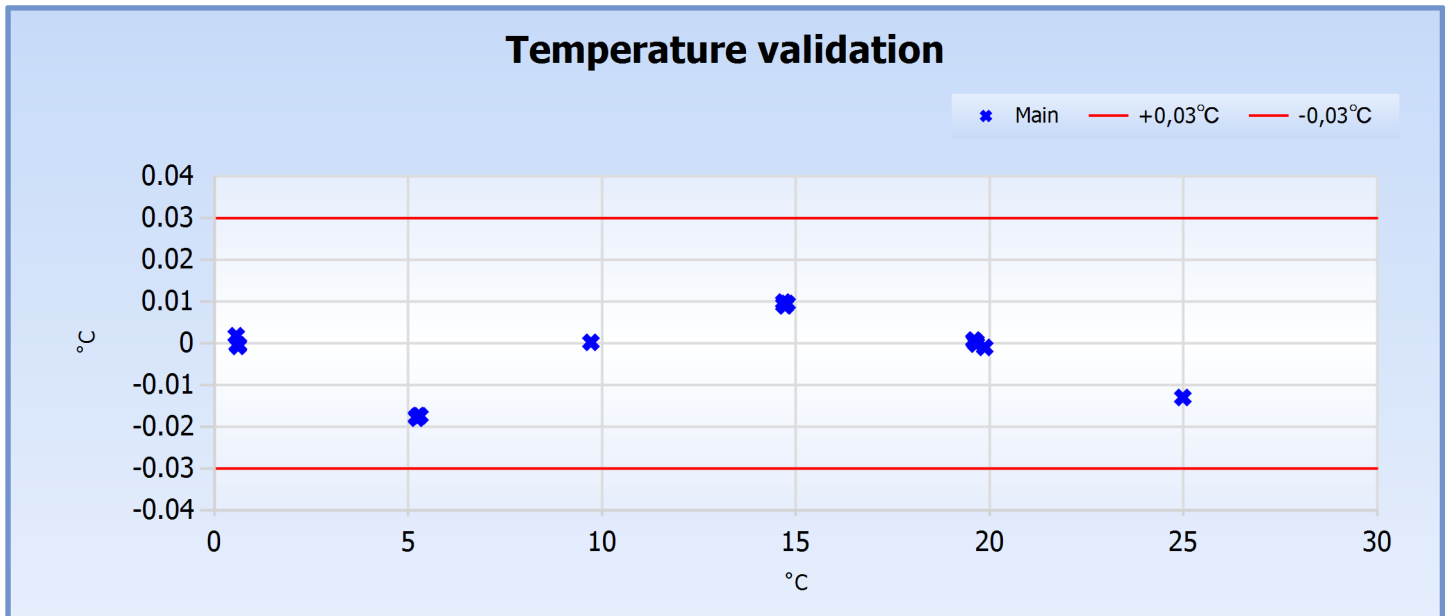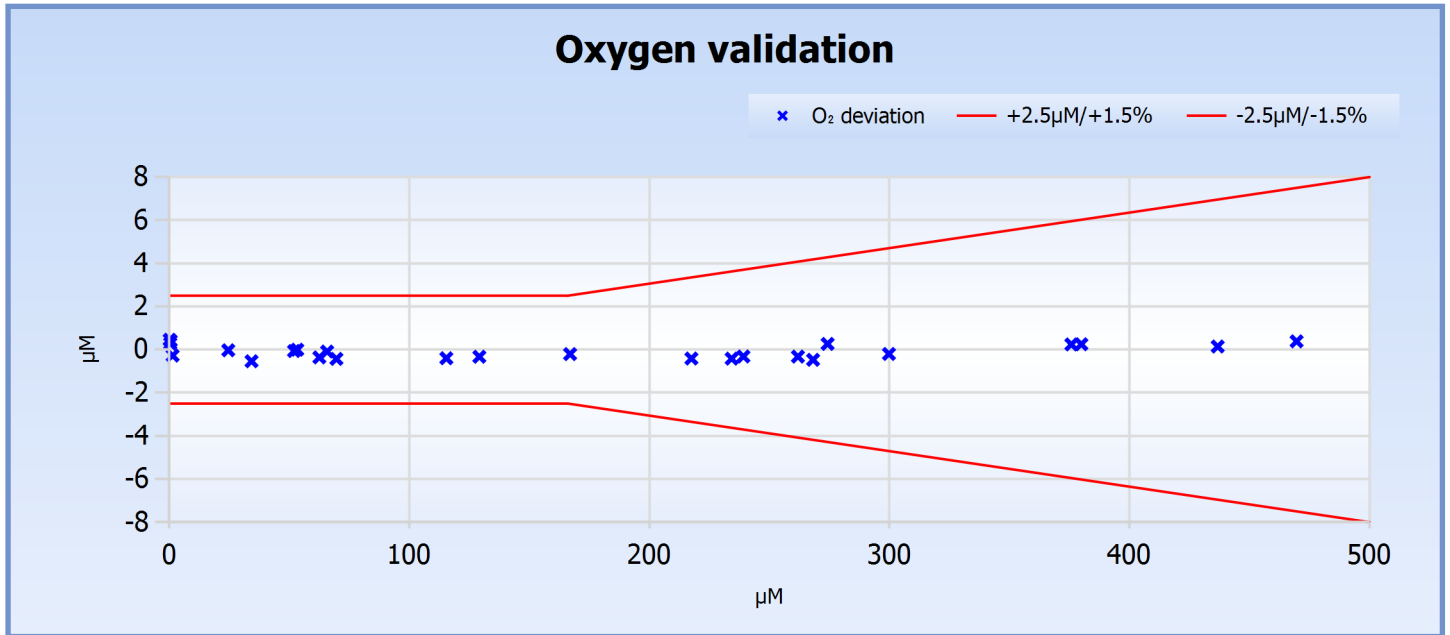

Date:14.01.2018

*Tor-Ove Kvalvaag*

Tor-Ove Kvalvaag, Calibration Engineer