

Certificate no: 4330_2976_00148637
Foil batch no: 1517MProduct: 4330
Calibration date: 31.05.2018Serial no: 2976
Page 1 of 2

Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.178	1.89	-115.800	60.32
1	20.131	1.61	207.493	61.25
2	10.311	1.62	525.433	62.00
3	0.882	1.97	809.100	62.66
4	1.077	20.46	803.560	60.10
5	1.227	42.36	799.333	57.40
6	1.424	63.72	793.727	55.00
7	1.537	107.81	790.567	50.82
8	1.575	147.74	789.473	47.65
9	1.604	216.12	788.633	43.34
10	1.641	321.02	787.567	38.41
11	1.646	425.79	787.433	34.84
12	1.666	524.29	786.827	32.25
13	10.680	18.58	513.700	58.81
14	10.557	34.28	517.647	56.03
15	10.527	51.05	518.587	53.46
16	10.528	85.54	518.567	49.08
17	10.521	119.54	518.787	45.57
18	10.489	169.00	519.800	41.51
19	10.459	252.00	520.760	36.56
20	10.429	335.48	521.713	33.04
21	10.416	419.84	522.100	30.39
22	20.469	15.50	196.427	57.51
23	20.331	28.43	200.927	54.47
24	20.255	41.07	203.427	51.86
25	20.227	69.07	204.307	47.17
26	20.226	96.43	204.387	43.54
27	20.242	137.38	203.820	39.31
28	20.255	202.05	203.393	34.53
29	20.261	269.70	203.200	31.06
30	20.268	341.97	202.973	28.41
31	30.092	13.24	-113.113	56.34
32	30.169	22.79	-115.520	53.28
33	30.236	34.86	-117.607	50.09
34	30.309	56.91	-119.900	45.35
35	30.372	79.39	-121.853	41.59
36	30.417	112.79	-123.253	37.35
37	30.434	166.73	-123.800	32.59
38	30.436	225.15	-123.800	29.16
39	30.417	281.32	-123.233	26.79



Certificate no: 4330_2976_00148637
 Foil batch no: 1517M

Product: 4330
 Calibration date: 31.05.2018

Serial no: 2976
 Page 2 of 2

Giving these coefficients

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.72357E-03	1.19420E-04	2.24266E-06	1.99716E02	-2.36344E-01	-4.04057E01	3.93834E00
TempCoef	2.65145E01	-3.12152E-02	3.09190E-06	-4.52265E-09	0.00000E00	0.00000E00	

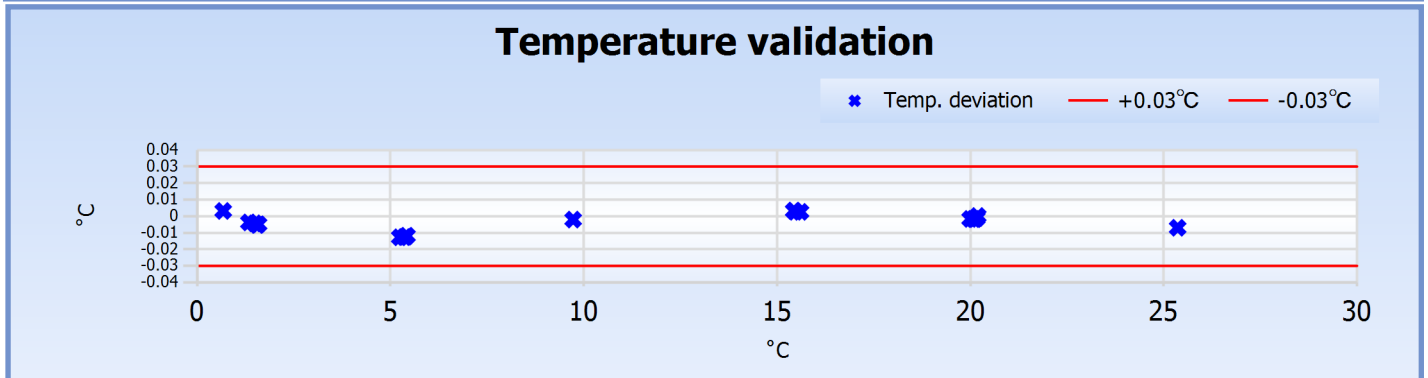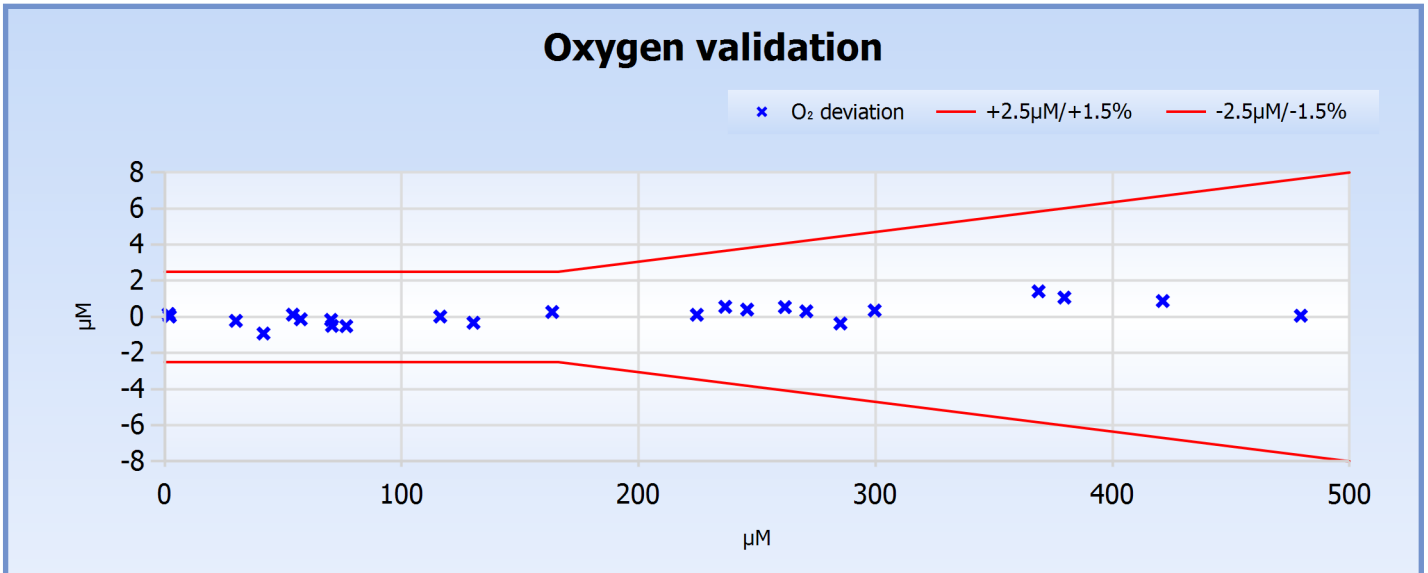

With following settings

Index	0 (Offset)	1 (Slope)
-------	------------	-----------

