

Certificate no: 4330\_2934\_00141932  
Foil batch no: 1517MProduct: 4330  
Calibration date: 14.01.2018Serial no: 2934  
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.285	0.22	-173.980	60.88
1	19.655	0.15	163.753	61.74
2	9.746	0.40	484.667	62.49
3	0.547	1.37	765.167	63.11
4	0.546	21.16	765.240	60.38
5	0.554	44.44	765.000	57.54
6	0.557	66.54	764.893	55.14
7	0.549	107.99	765.173	51.27
8	0.551	151.57	765.080	47.91
9	0.559	225.26	764.880	43.39
10	0.567	324.05	764.627	38.87
11	0.572	434.00	764.513	35.18
12	0.574	549.08	764.413	32.29
13	10.095	12.98	473.620	59.98
14	10.023	32.51	475.893	56.53
15	9.965	49.91	477.707	53.86
16	9.924	83.85	479.053	49.50
17	9.886	116.44	480.240	46.12
18	9.857	172.96	481.167	41.54
19	9.834	252.02	481.920	36.89
20	9.823	335.47	482.280	33.37
21	9.821	420.40	482.320	30.69
22	19.840	9.48	157.780	59.14
23	19.771	24.28	160.027	55.47
24	19.715	37.79	161.833	52.60
25	19.676	64.90	163.093	47.89
26	19.651	93.02	163.907	44.06
27	19.626	136.26	164.720	39.57
28	19.603	201.45	165.500	34.79
29	19.593	267.50	165.800	31.43
30	19.592	336.88	165.833	28.82
31	29.979	7.38	-164.587	58.16
32	29.983	19.64	-164.700	54.04
33	29.987	30.64	-164.827	50.95
34	29.991	51.88	-164.933	46.14
35	29.993	73.64	-165.013	42.33
36	29.990	109.72	-164.913	37.62
37	29.995	163.46	-165.080	32.85
38	30.001	218.96	-165.253	29.51
39	30.002	276.10	-165.280	27.05

Certificate no: 4330\_2934\_00141932  
Foil batch no: 1517M

Product: 4330  
Calibration date: 14.01.2018

Serial no: 2934  
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.80945E-03	1.18493E-04	2.43592E-06	7.72232E01	-1.16629E-01	-1.89134E01	1.52484E00
TempCoef	2.47241E01	-3.13203E-02	2.97469E-06	-4.35741E-09	0.00000E00	0.00000E00	

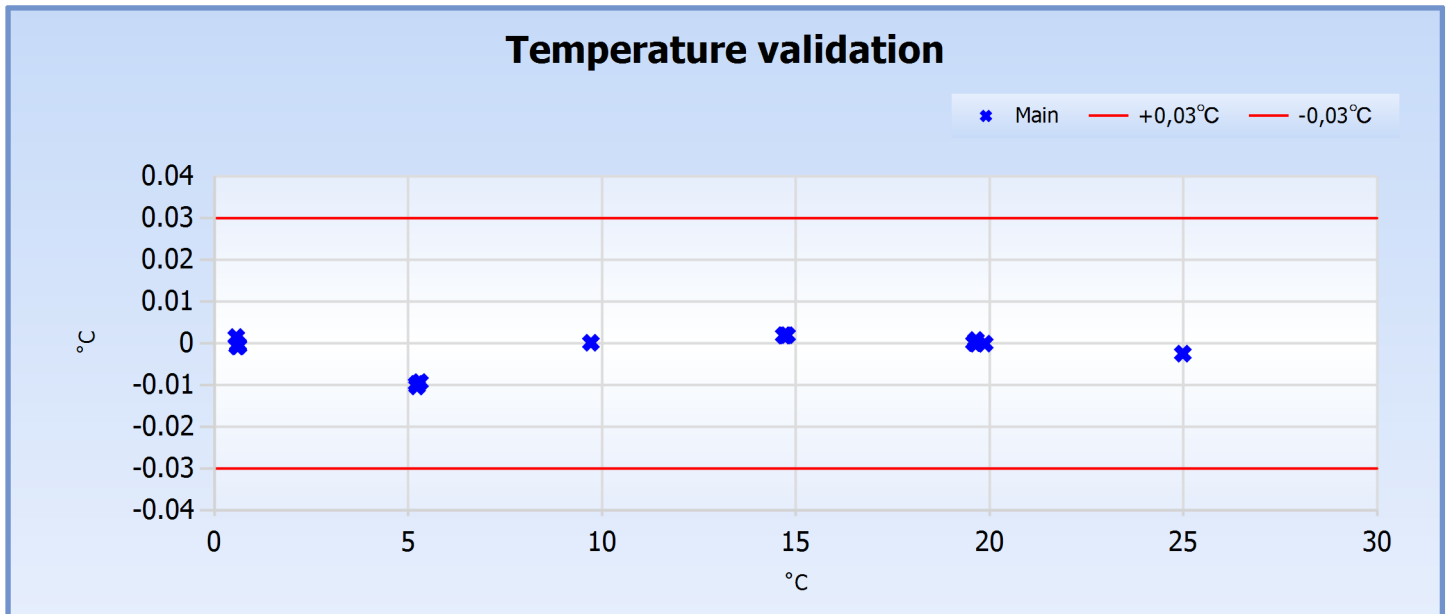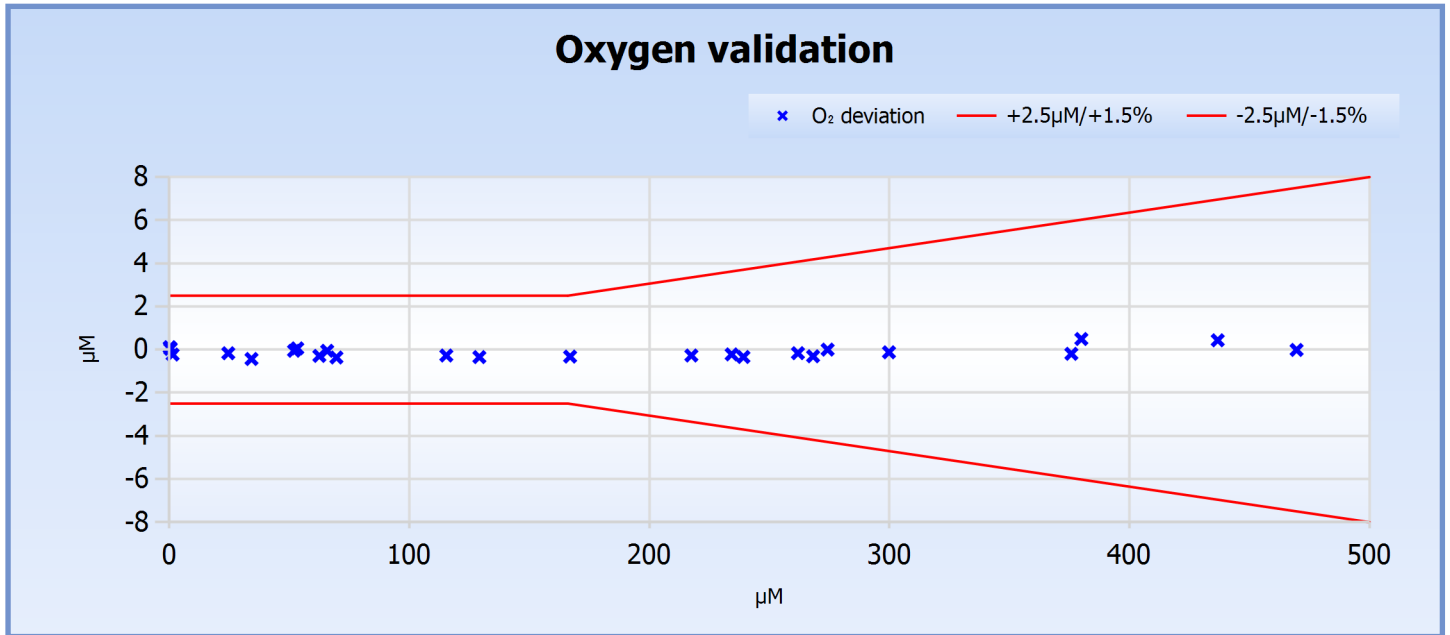

Date:14.01.2018

*Tor-Ove Kvalvaag*

Tor-Ove Kvalvaag, Calibration Engineer