



Certificate no: 4330\_2906\_00137202  
Foil batch no: 1517M

Product: 4330  
Calibration date: 13.11.2017

Serial no: 2906  
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.81697E-03	1.18333E-04	2.37322E-06	1.14293E02	-2.09054E-01	-2.79017E01	2.26782E00
TempCoef	2.43116E01	-3.06145E-02	2.81432E-06	-4.23068E-09	0.00000E00	0.00000E00	

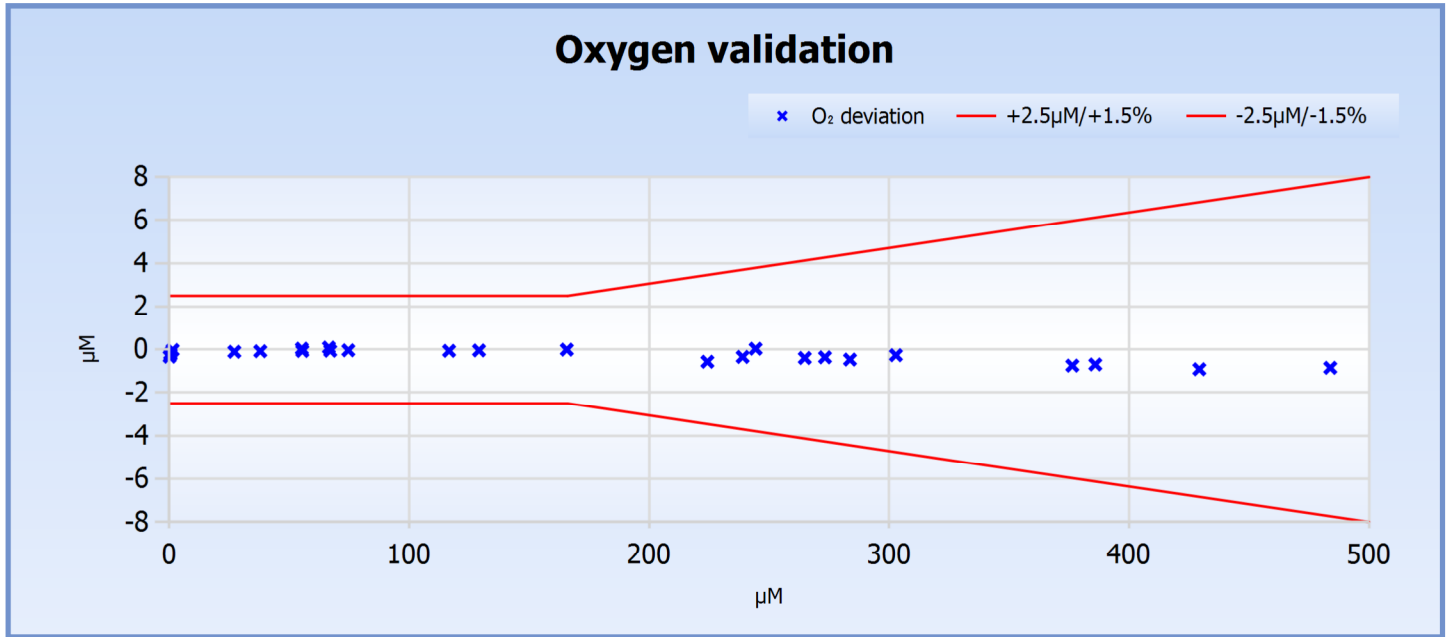

Date:13.11.2017

*Tor-Ove Kvalvaag*  
Tor-Ove Kvalvaag, Calibration Engineer

Certificate no: 4330\_2907\_00137200  
Foil batch no: 1517MProduct: 4330  
Calibration date: 13.11.2017Serial no: 2907  
Page 1 of 2

Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	29.911	0.75	-217.200	60.66
1	20.131	0.28	98.213	61.75
2	10.326	0.47	424.420	62.56
3	0.836	1.42	725.113	63.27
4	0.913	22.62	722.800	60.35
5	0.987	44.02	720.547	57.69
6	1.016	65.31	719.673	55.34
7	1.034	106.92	719.120	51.39
8	1.064	149.42	718.233	48.05
9	1.083	213.13	717.673	44.02
10	1.119	317.20	716.560	39.09
11	1.149	421.85	715.693	35.51
12	1.172	527.65	715.000	32.76
13	10.315	15.63	424.787	59.56
14	10.199	34.09	428.653	56.35
15	10.134	50.90	430.753	53.81
16	10.107	83.81	431.673	49.61
17	10.092	117.59	432.133	46.12
18	10.082	168.06	432.453	42.00
19	10.074	250.83	432.720	37.09
20	10.100	334.30	431.900	33.55
21	10.086	418.92	432.327	30.91
22	20.071	12.03	100.193	58.39
23	19.970	26.68	103.553	54.88
24	19.933	40.15	104.780	52.12
25	19.916	66.41	105.400	47.67
26	19.912	93.37	105.500	44.05
27	19.914	133.60	105.400	39.87
28	19.925	199.94	105.073	34.98
29	19.931	267.71	104.867	31.53
30	19.940	336.41	104.593	28.99
31	29.963	9.40	-218.767	57.23
32	29.966	21.33	-218.893	53.40
33	29.998	32.35	-219.867	50.44
34	30.024	53.86	-220.687	45.76
35	30.042	75.83	-221.213	42.06
36	30.054	108.90	-221.600	37.84
37	30.063	163.33	-221.880	33.05
38	30.068	219.35	-222.000	29.72
39	30.071	277.09	-222.100	27.27