

Certificate no: 4330_2903_00137192
Foil batch no: 1517MProduct: 4330
Calibration date: 13.11.2017Serial no: 2903
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	29.911	0.75	-203.320	60.49
1	20.131	0.28	112.613	61.64
2	10.326	0.47	438.340	62.47
3	0.836	1.42	737.447	63.18
4	0.913	22.62	735.167	60.27
5	0.987	44.02	732.920	57.63
6	1.016	65.31	732.040	55.27
7	1.034	106.92	731.513	51.33
8	1.064	149.42	730.620	48.00
9	1.083	213.13	730.027	43.97
10	1.119	317.20	728.947	39.06
11	1.149	421.85	728.027	35.48
12	1.172	527.65	727.380	32.73
13	10.315	15.63	438.667	59.45
14	10.199	34.09	442.473	56.28
15	10.134	50.90	444.573	53.76
16	10.107	83.81	445.487	49.57
17	10.092	117.59	445.980	46.08
18	10.082	168.06	446.293	41.96
19	10.074	250.83	446.573	37.05
20	10.100	334.30	445.707	33.52
21	10.086	418.92	446.187	30.88
22	20.071	12.03	114.600	58.28
23	19.970	26.68	117.933	54.80
24	19.933	40.15	119.173	52.06
25	19.916	66.41	119.767	47.62
26	19.912	93.37	119.900	44.01
27	19.914	133.60	119.800	39.83
28	19.925	199.94	119.447	34.94
29	19.931	267.71	119.213	31.50
30	19.940	336.41	118.947	28.95
31	29.963	9.40	-204.920	57.09
32	29.966	21.33	-205.047	53.31
33	29.998	32.35	-206.007	50.37
34	30.024	53.86	-206.827	45.72
35	30.042	75.83	-207.380	42.03
36	30.054	108.90	-207.773	37.81
37	30.063	163.33	-208.027	33.02
38	30.068	219.35	-208.207	29.69
39	30.071	277.09	-208.287	27.24

Certificate no: 4330_2903_00137192
Foil batch no: 1517M

Product: 4330
Calibration date: 13.11.2017

Serial no: 2903
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.80898E-03	1.17750E-04	2.39215E-06	1.25352E02	-2.27661E-01	-3.14673E01	2.48711E00
TempCoef	2.35445E01	-3.05747E-02	2.77781E-06	-4.16717E-09	0.00000E00	0.00000E00	

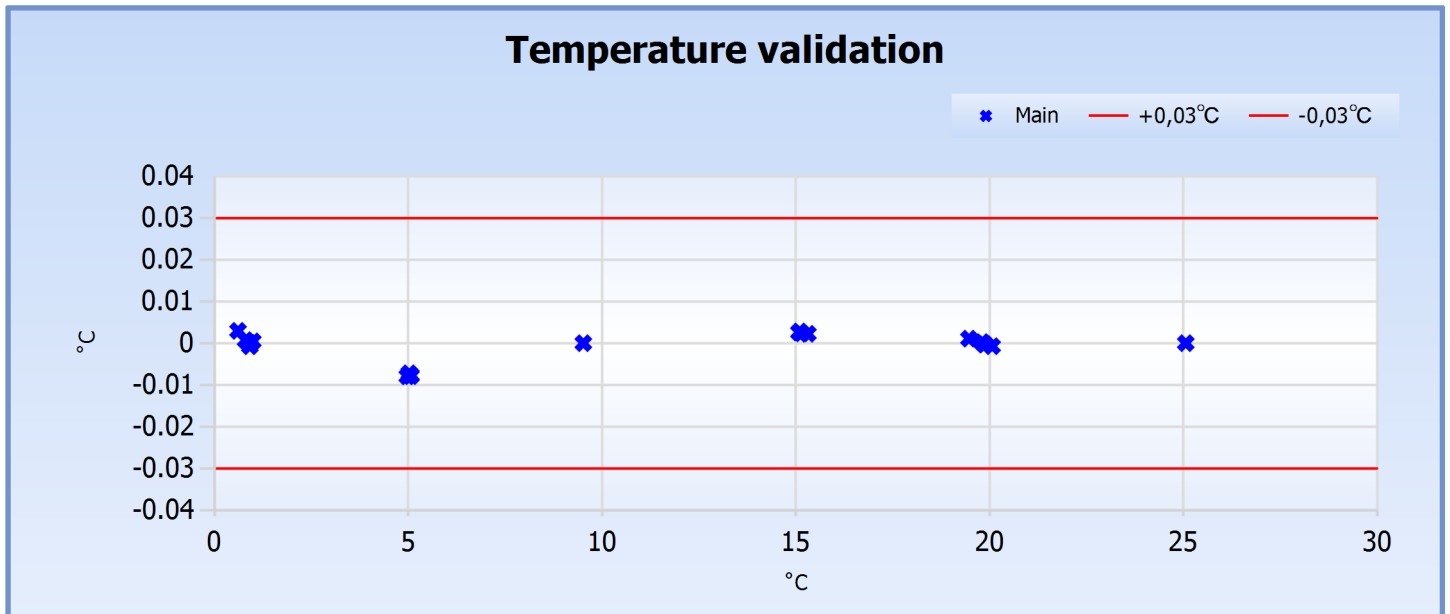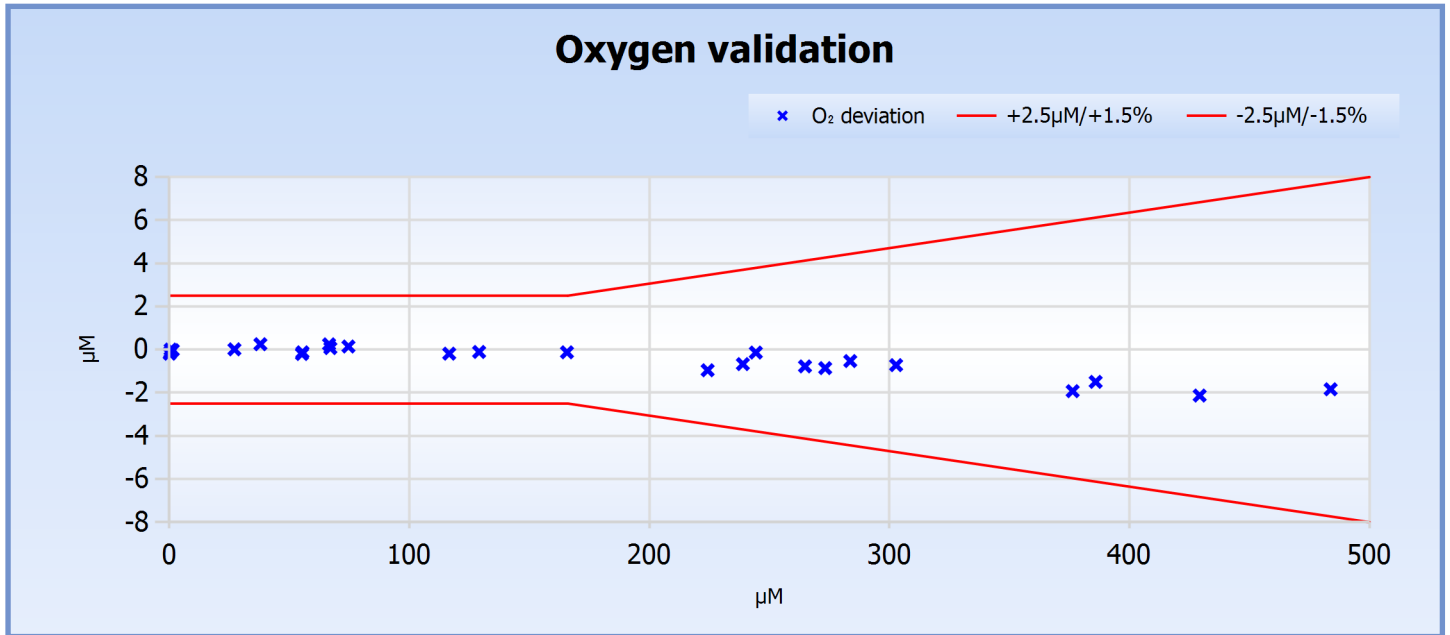

Date:13.11.2017

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer