

Certificate no: 4330_2932_00141948
Foil batch no: 1517M

Product: 4330
Calibration date: 14.01.2018

Serial no: 2932
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.285	0.22	-97.887	61.90
1	19.655	0.15	246.067	62.80
2	9.746	0.40	565.807	63.59
3	0.547	1.37	838.927	64.27
4	0.546	21.16	838.973	61.51
5	0.554	44.44	838.773	58.65
6	0.557	66.54	838.693	56.24
7	0.549	107.99	838.940	52.34
8	0.551	151.57	838.833	48.96
9	0.559	225.26	838.653	44.41
10	0.567	324.05	838.400	39.89
11	0.572	434.00	838.247	36.20
12	0.574	549.08	838.207	33.32
13	10.095	12.98	554.907	61.09
14	10.023	32.51	557.173	57.60
15	9.965	49.91	558.960	54.92
16	9.924	83.85	560.267	50.54
17	9.886	116.44	561.413	47.14
18	9.857	172.96	562.360	42.53
19	9.834	252.02	563.067	37.88
20	9.823	335.47	563.427	34.37
21	9.821	420.40	563.487	31.71
22	19.840	9.48	240.020	60.19
23	19.771	24.28	242.307	56.49
24	19.715	37.79	244.133	53.61
25	19.676	64.90	245.413	48.88
26	19.651	93.02	246.220	45.03
27	19.626	136.26	247.027	40.53
28	19.603	201.45	247.800	35.76
29	19.593	267.50	248.107	32.40
30	19.592	336.88	248.127	29.79
31	29.979	7.38	-88.287	59.15
32	29.983	19.64	-88.400	55.01
33	29.987	30.64	-88.540	51.90
34	29.991	51.88	-88.647	47.06
35	29.993	73.64	-88.727	43.25
36	29.990	109.72	-88.627	38.54
37	29.995	163.46	-88.793	33.77
38	30.001	218.96	-88.973	30.43
39	30.002	276.10	-89.007	27.98

Certificate no: 4330_2932_00141948
 Foil batch no: 1517M

Product: 4330
 Calibration date: 14.01.2018

Serial no: 2932
 Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.82887E-03	1.18839E-04	2.54255E-06	1.51871E02	-2.37720E-01	-3.79960E01	2.99528E00
TempCoef	2.71992E01	-3.11651E-02	3.22089E-06	-4.69575E-09	0.00000E00	0.00000E00	

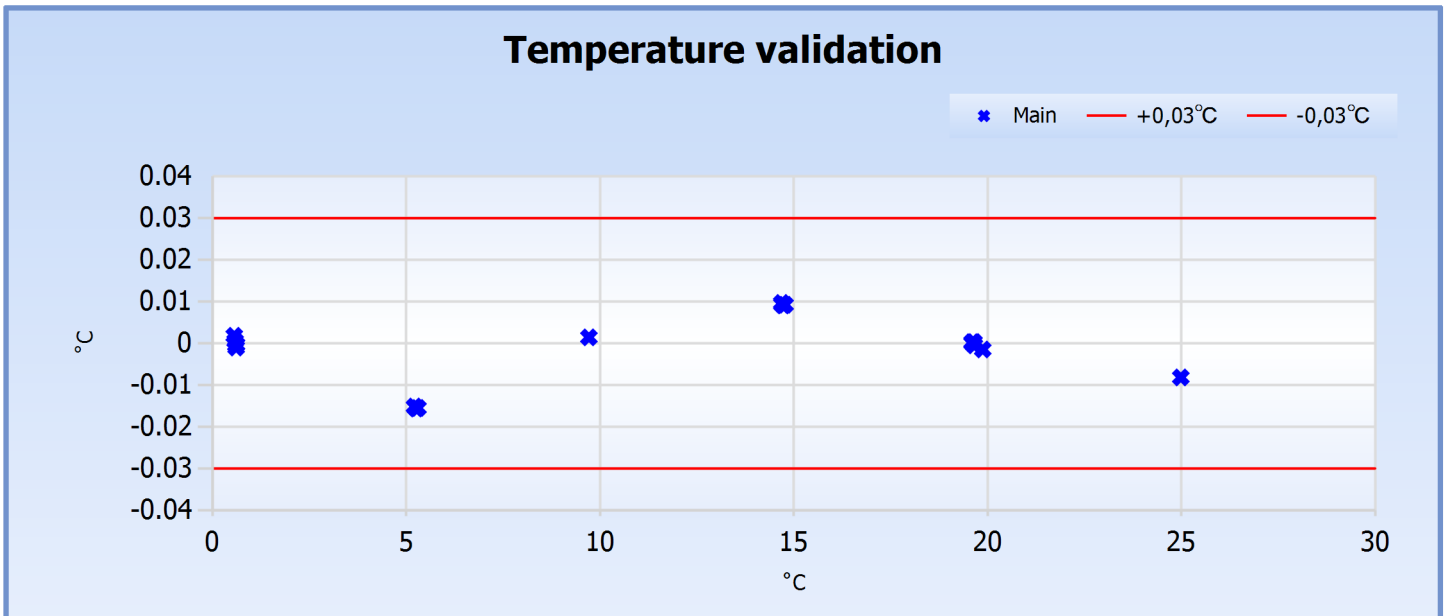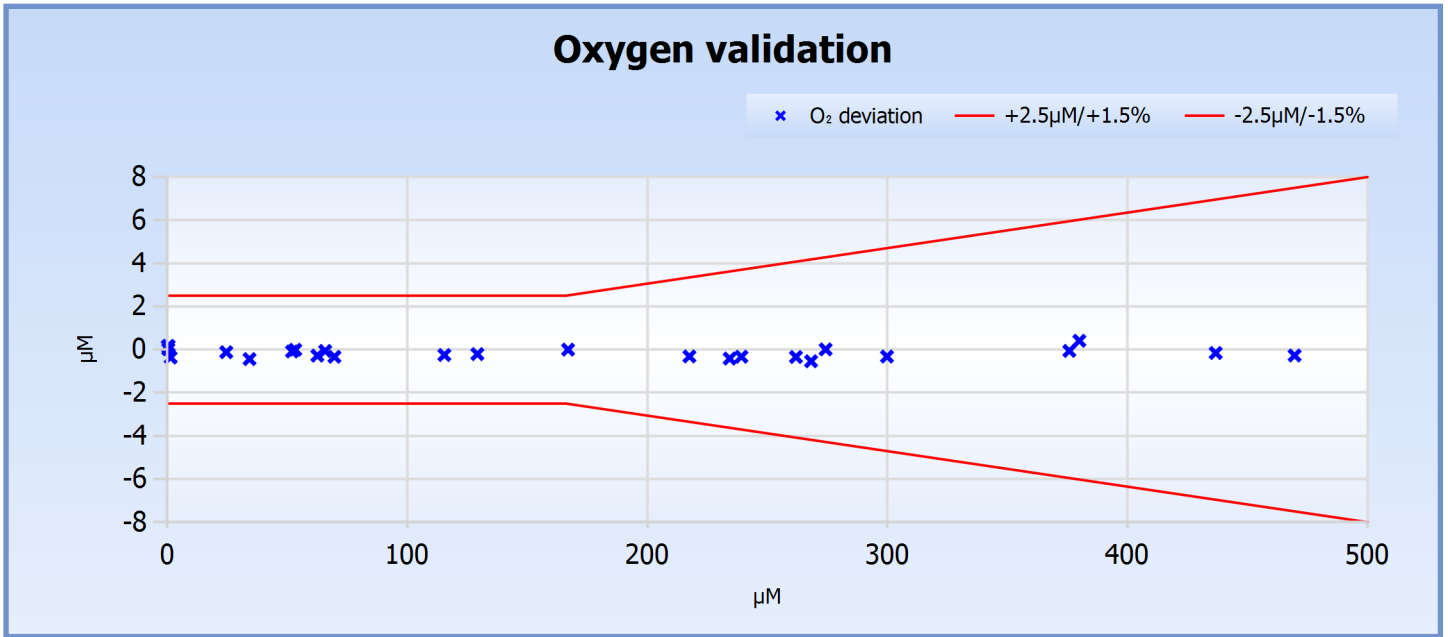

Date:14.01.2018

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer