

Certificate no: 4330_2945_00146791
Foil batch no: 1517M

Product: 4330
Calibration date: 12.04.2018

Serial no: 2945
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.195	1.84	-34.613	59.73
1	20.092	1.50	291.433	60.78
2	10.245	1.48	604.527	61.50
3	0.831	1.84	877.180	62.09
4	0.877	19.96	875.940	59.66
5	0.919	41.92	874.793	57.00
6	0.950	64.32	873.940	54.57
7	0.980	104.55	873.180	50.78
8	1.017	150.41	872.133	47.19
9	1.055	217.74	871.167	42.97
10	1.113	325.76	869.587	37.98
11	1.144	425.27	868.813	34.59
12	1.152	535.16	868.573	31.74
13	10.671	19.34	591.567	58.08
14	10.491	33.93	597.100	55.60
15	10.411	51.93	599.533	52.89
16	10.343	85.64	601.627	48.61
17	10.297	117.99	603.047	45.29
18	10.272	171.47	603.807	40.93
19	10.245	254.41	604.620	36.03
20	10.212	340.06	605.647	32.46
21	10.184	427.65	606.493	29.79
22	20.474	16.49	279.100	56.71
23	20.383	28.73	282.013	53.89
24	20.324	41.75	283.953	51.27
25	20.269	68.70	285.720	46.74
26	20.235	94.58	286.800	43.28
27	20.228	137.58	287.027	38.82
28	20.222	203.07	287.200	34.01
29	20.220	272.52	287.313	30.50
30	20.218	340.77	287.340	27.99
31	30.165	14.28	-33.607	55.46
32	30.175	23.63	-33.947	52.61
33	30.200	34.51	-34.727	49.76
34	30.227	56.40	-35.573	45.06
35	30.255	78.87	-36.460	41.29
36	30.275	113.00	-37.093	36.95
37	30.290	168.27	-37.580	32.13
38	30.306	225.58	-38.087	28.75
39	30.320	281.89	-38.493	26.39

Certificate no: 4330_2945_00146791
 Foil batch no: 1517M

Product: 4330
 Calibration date: 12.04.2018

Serial no: 2945
 Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.73212E-03	1.19724E-04	2.15378E-06	1.76275E02	-2.11627E-01	-4.07478E01	3.48118E00
TempCoef	2.91003E01	-3.15265E-02	3.58179E-06	-4.99126E-09	0.00000E00	0.00000E00	

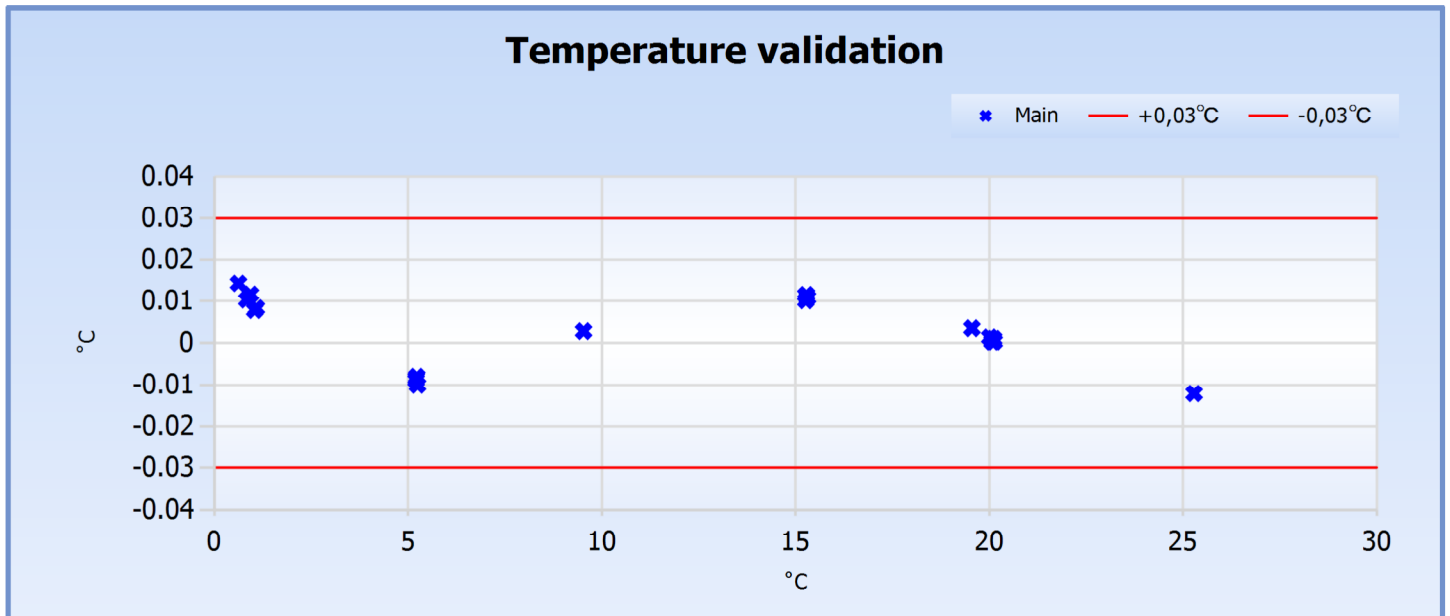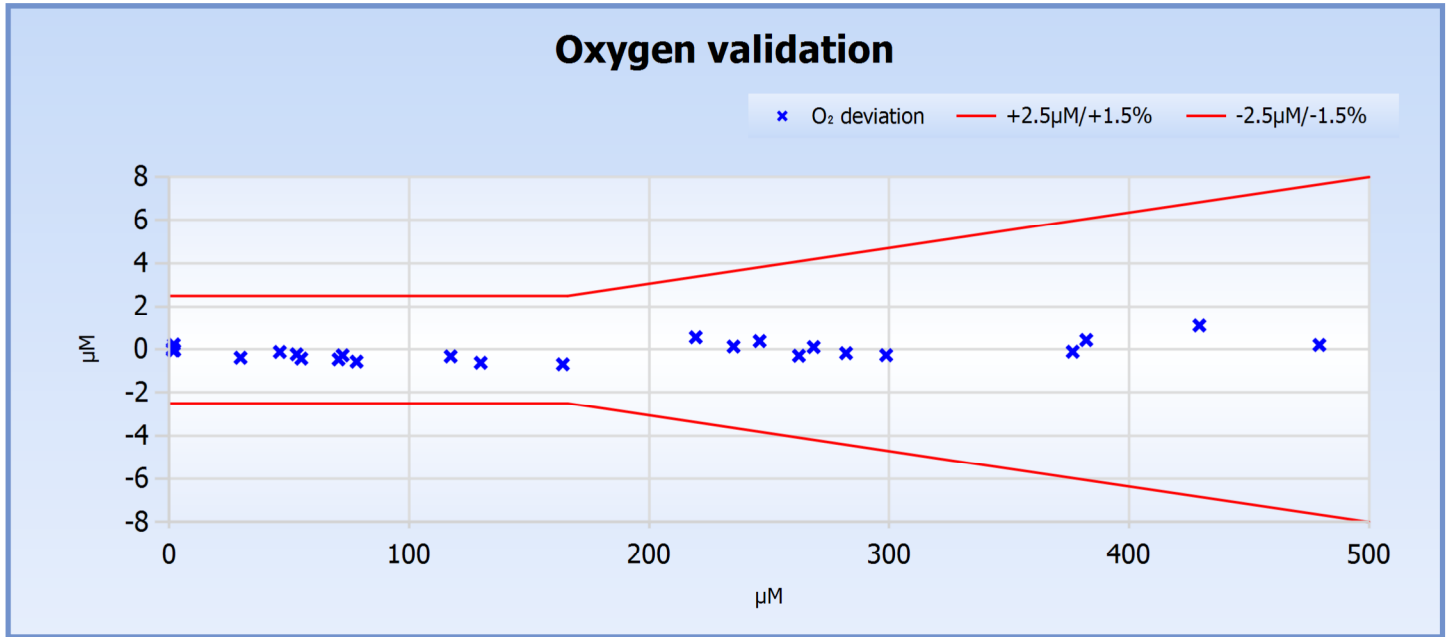

Date:12.04.2018


 Tor-Ove Kvalvaag, Calibration Engineer