

Certificate no: 4330_2947_00146792
Foil batch no: 1517M

Product: 4330
Calibration date: 12.04.2018

Serial no: 2947
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.195	1.84	-105.927	60.12
1	20.092	1.50	216.707	61.19
2	10.245	1.48	532.487	61.93
3	0.831	1.84	812.760	62.57
4	0.877	19.96	811.480	60.14
5	0.919	41.92	810.273	57.49
6	0.950	64.32	809.467	55.07
7	0.980	104.55	808.600	51.30
8	1.017	150.41	807.547	47.75
9	1.055	217.74	806.487	43.57
10	1.113	325.76	804.873	38.58
11	1.144	425.27	804.007	35.20
12	1.152	535.16	803.800	32.34
13	10.671	19.34	519.147	58.58
14	10.491	33.93	524.773	56.09
15	10.411	51.93	527.260	53.39
16	10.343	85.64	529.413	49.15
17	10.297	117.99	530.847	45.84
18	10.272	171.47	531.620	41.50
19	10.245	254.41	532.453	36.61
20	10.212	340.06	533.493	33.04
21	10.184	427.65	534.373	30.36
22	20.474	16.49	204.347	57.26
23	20.383	28.73	207.273	54.40
24	20.324	41.75	209.193	51.76
25	20.269	68.70	210.980	47.23
26	20.235	94.58	212.100	43.78
27	20.228	137.58	212.293	39.33
28	20.222	203.07	212.493	34.54
29	20.220	272.52	212.587	31.03
30	20.218	340.77	212.600	28.52
31	30.165	14.28	-105.000	55.89
32	30.175	23.63	-105.287	53.02
33	30.200	34.51	-106.060	50.14
34	30.227	56.40	-106.900	45.45
35	30.255	78.87	-107.767	41.71
36	30.275	113.00	-108.393	37.39
37	30.290	168.27	-108.867	32.58
38	30.306	225.58	-109.367	29.23
39	30.320	281.89	-109.780	26.87

Certificate no: 4330_2947_00146792
 Foil batch no: 1517M

Product: 4330
 Calibration date: 12.04.2018

Serial no: 2947
 Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.70554E-03	1.18264E-04	2.22868E-06	1.66475E02	-2.03216E-01	-3.83232E01	3.29088E00
TempCoef	2.68177E01	-3.15004E-02	3.14652E-06	-4.58441E-09	0.00000E00	0.00000E00	

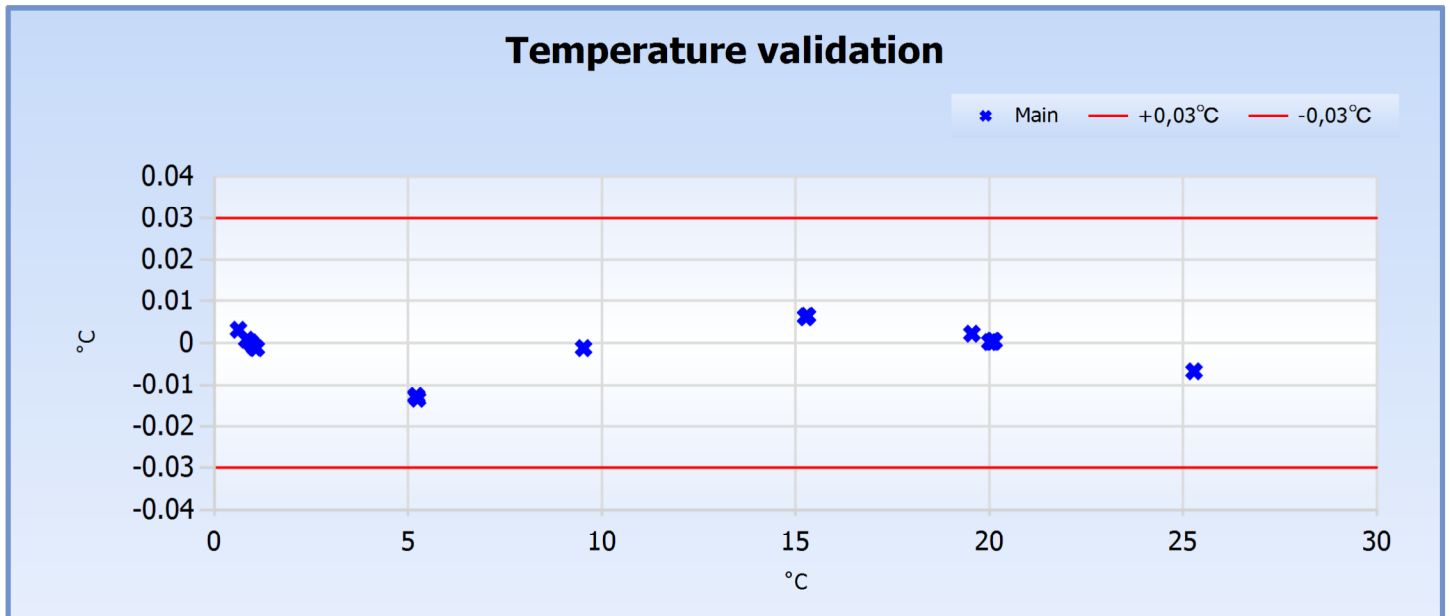

Date:12.04.2018

Tor-Ove Kvalvaag
 Tor-Ove Kvalvaag, Calibration Engineer