



a xylem brand

CALIBRATION CERTIFICATE

Form No 830, Juli 2012

Certificate no: 4330_1466_00140825
Foil batch no: 1206EM

Product: 4330
Calibration date: 13.12.2017

Serial no: 1466
Page 1 of 2



Index	Temperature reference(°C)	[O2] Reference(µM)	Temperature raw data(mV)	Phase reading(°)
0	30.037	0.62	-135.313	62.15
1	20.049	0.36	190.840	63.02
2	10.156	0.65	517.520	63.77
3	0.788	1.84	805.467	64.40
4	0.774	21.17	805.860	61.50
5	0.768	42.48	805.973	58.64
6	0.758	64.75	806.333	56.00
7	0.750	105.61	806.553	51.87
8	0.770	146.53	805.967	48.46
9	0.787	213.54	805.473	44.01
10	0.798	315.73	805.160	39.03
11	0.808	423.27	804.853	35.29
12	0.814	528.00	804.680	32.54
13	10.211	17.81	515.767	60.19
14	10.167	34.30	517.227	57.10
15	10.133	50.44	518.300	54.45
16	10.113	82.63	518.907	50.01
17	10.073	114.96	520.233	46.43
18	10.056	166.89	520.773	41.97
19	10.049	249.58	521.000	36.89
20	10.046	332.33	521.087	33.32
21	10.047	415.99	521.060	30.67
22	20.388	14.77	179.580	58.77
23	20.253	26.74	184.033	55.67
24	20.190	39.61	186.133	52.79
25	20.131	65.36	188.087	48.07
26	20.058	91.20	190.507	44.36
27	20.023	132.38	191.667	39.86
28	20.003	197.55	192.360	34.88
29	19.987	264.82	192.880	31.39
30	19.973	333.51	193.353	28.82
31	30.070	11.89	-136.327	57.73
32	30.054	21.88	-135.840	54.29
33	30.064	32.41	-136.167	51.20
34	30.082	53.53	-136.700	46.25
35	30.097	75.41	-137.200	42.32
36	30.107	108.23	-137.520	37.92
37	30.114	161.44	-137.733	33.05
38	30.120	217.52	-137.900	29.64
39	30.120	274.32	-137.900	27.19

Certificate no: 4330_1466_00140825
Foil batch no: 1206EM

Product: 4330
Calibration date: 13.12.2017

Serial no: 1466
Page 2 of 2

Index	0	1	2	3	4	5	6
SVUFoilCoef	3.03932E-03	1.28563E-04	2.50282E-06	1.13786E02	-1.66689E-01	-2.77584E01	2.20632E00
TempCoef	2.58198E01	-3.06684E-02	3.09421E-06	-4.47314E-09	0.00000E00	0.00000E00	

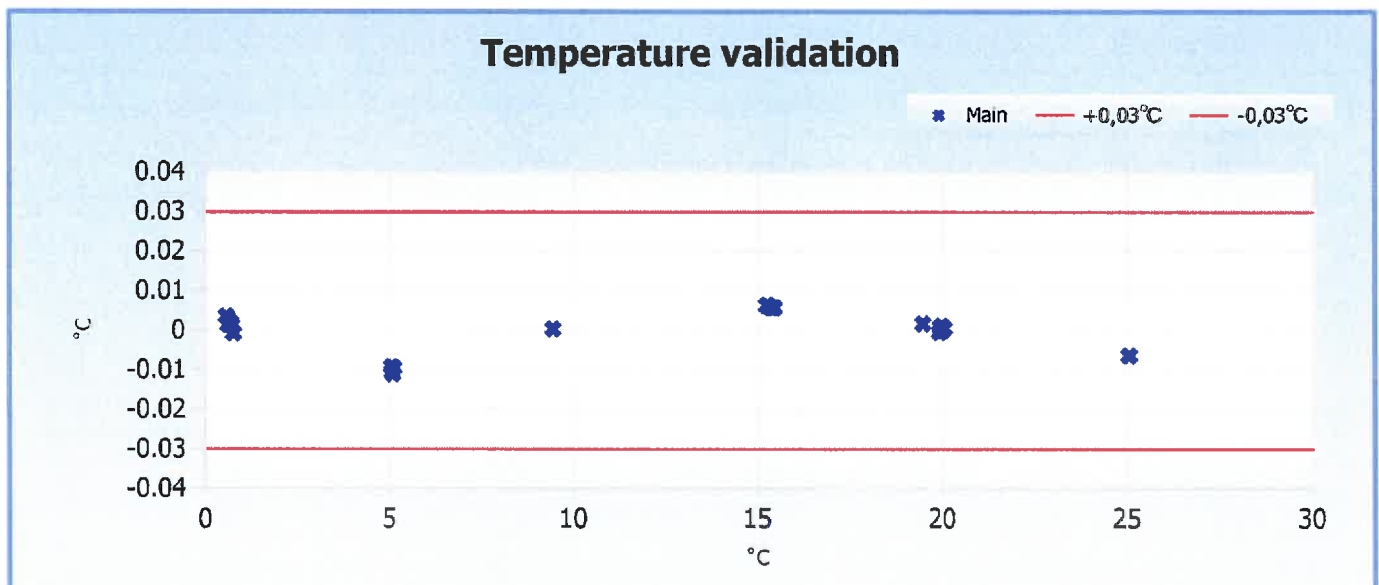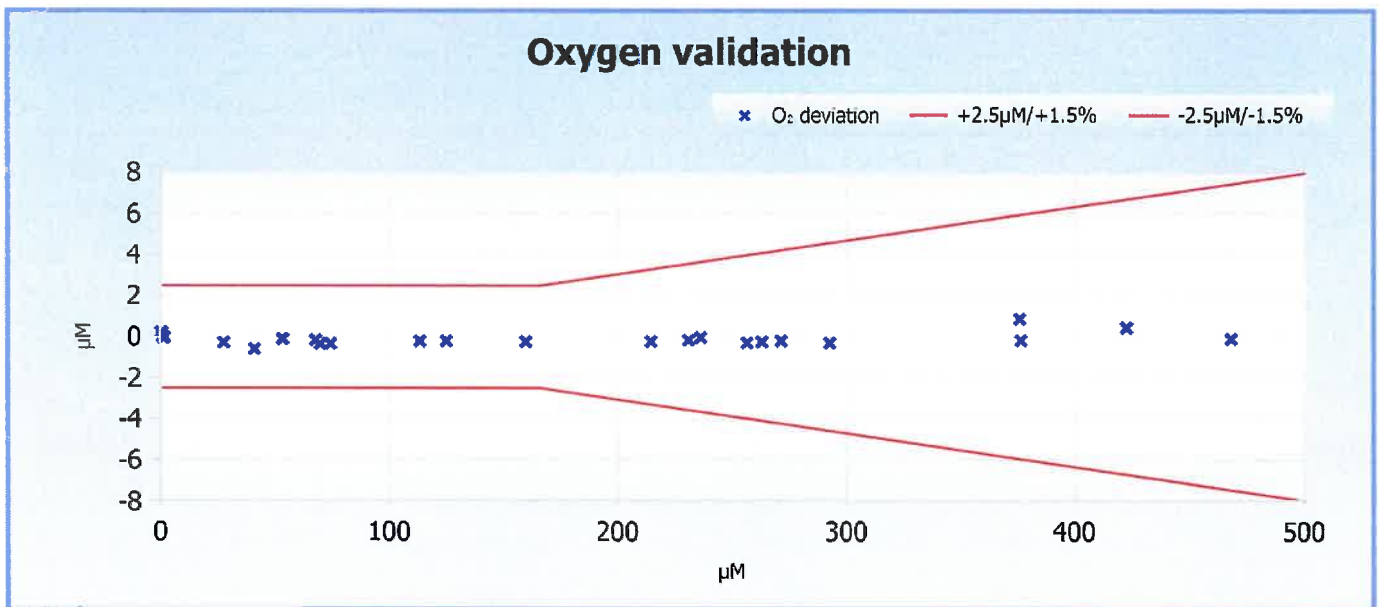

Date: 13.12.2017

Tor-Ove Kvalvaag
Tor-Ove Kvalvaag, Calibration Engineer